


Mass Spectrum

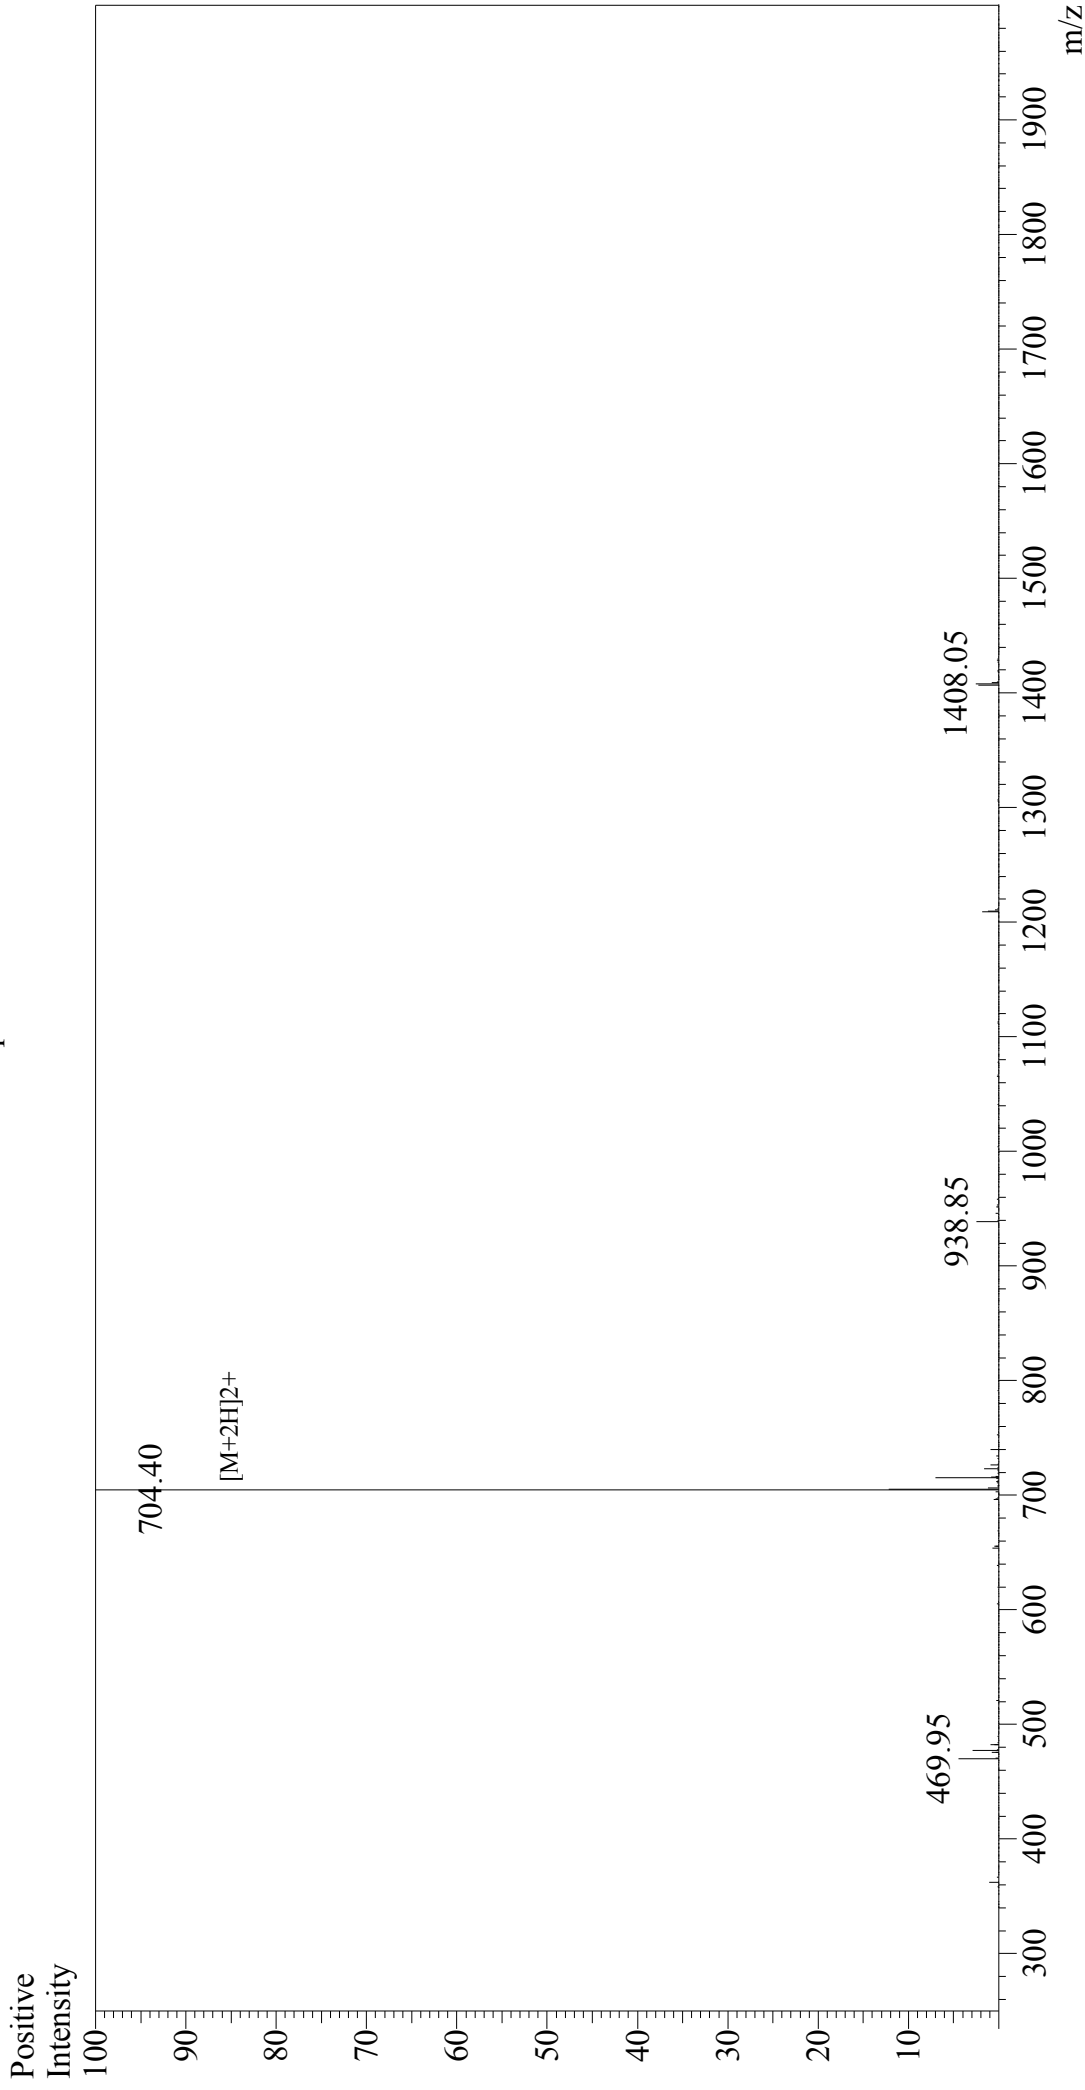

Sample Information

Acquired by : Gary
Month-Day Processed : 05/11/18
Time Processed : 9:44:30
Injection Volume : 0.2
Sample Name : Hepatitis B Virus Core (128-140)
Cat. No. : RP17313
Lot. No. : PE7611805
Theoretical MW : 1406.63
Observed MW : 1406.80

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H₂O/50% MeOH