

Sample Name :CEF14, EBV Rta Protein (28-37)
 Cat No. :RP20442
 Lot No. :E7324521C
 Time Processed :14:58:45
 Month-Day-Year Processed :03/20/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

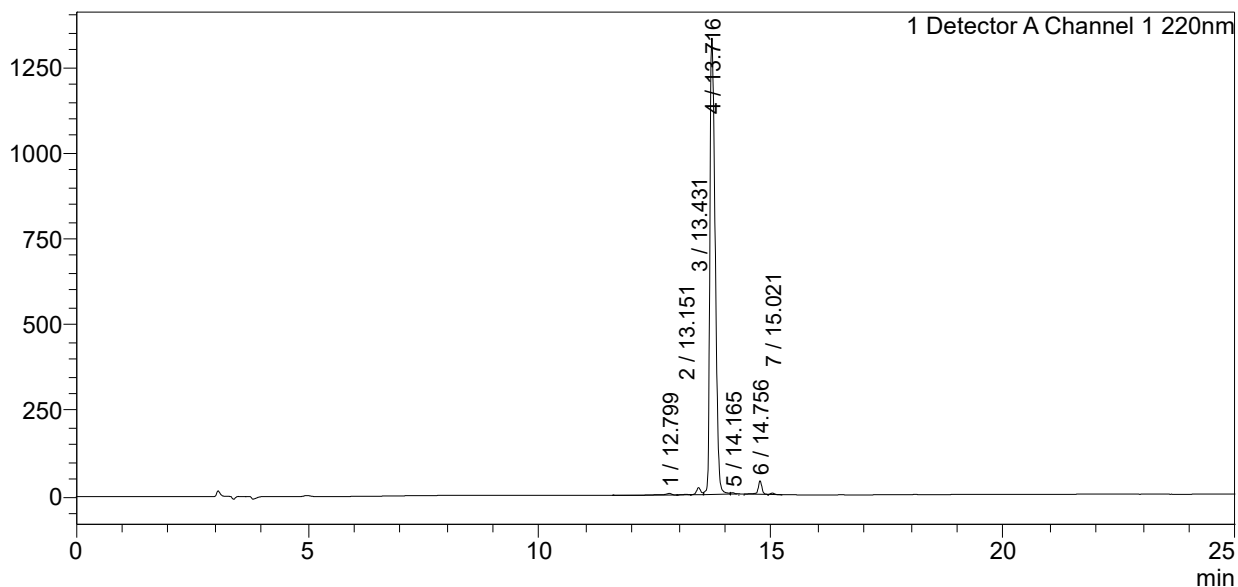

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.799	44927	4656	0.407
2	13.151	12756	1733	0.116
3	13.431	127997	20748	1.159
4	13.716	10576814	1329629	95.799
5	14.165	27279	4362	0.247
6	14.756	225505	39284	2.043
7	15.021	25300	4321	0.229
Total		11040578	1404733	100.000