

Sample Name: Arg-Gly-Asp-Cys
 Cat No.: RP10860
 Lot No.: E6031120C
 Time Processed: 11:10:54 AM
 Month-Day-Year Processed: 03/28/2020

Pump A: 0.065% trifluoroacetic in 100% water (v/v)
 Pump B: 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column: Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

mV

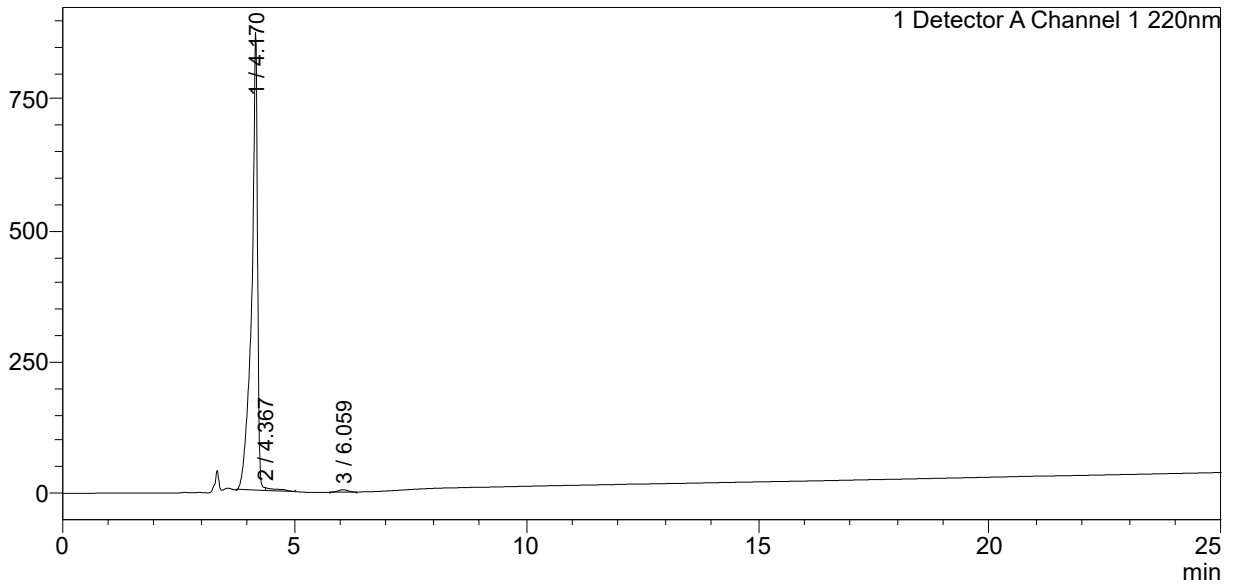

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	4.170	7608129	870896	97.815
2	4.367	102367	5385	1.316
3	6.059	67571	4640	0.869
Total		7778067	880920	100.000