

Sample Name : SIYRY
 Cat. No. : RP20234
 Lot. No. : PE4861711

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

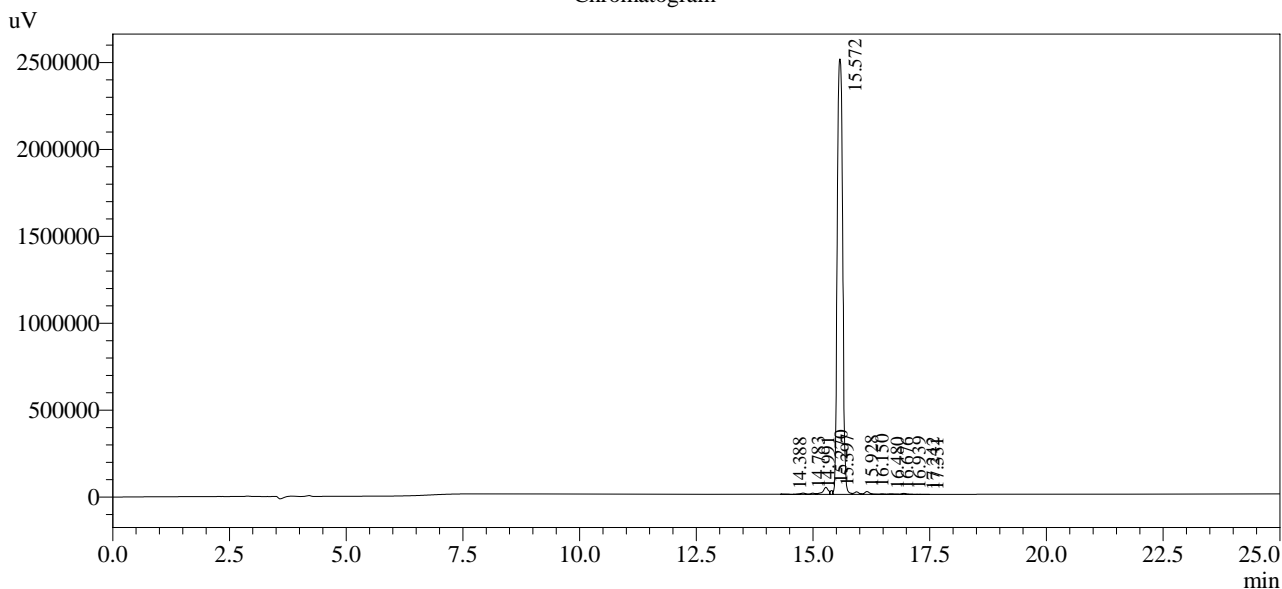

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.388	4373	820	0.021
2	14.783	60202	7227	0.288
3	14.991	42250	6871	0.202
4	15.270	320953	40098	1.538
5	15.397	80311	21386	0.385
6	15.572	20041670	2505098	96.036
7	15.928	99092	14260	0.475
8	16.150	126041	16066	0.604
9	16.480	18926	2565	0.091
10	16.676	30484	2809	0.146
11	16.939	42545	5607	0.204
12	17.242	658	181	0.003
13	17.331	1514	200	0.007
Total		20869018	2623188	100.000