

Sample Name :Arg-Gly-Asp-Ser
 Cat No. :RP10861
 Lot No. :E9404421D
 Time Processed : 9:59:07 PM
 Month-Day-Year Processed : 04/27/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
32.00	Pumps	B.Conc	95
32.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
45.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

mV

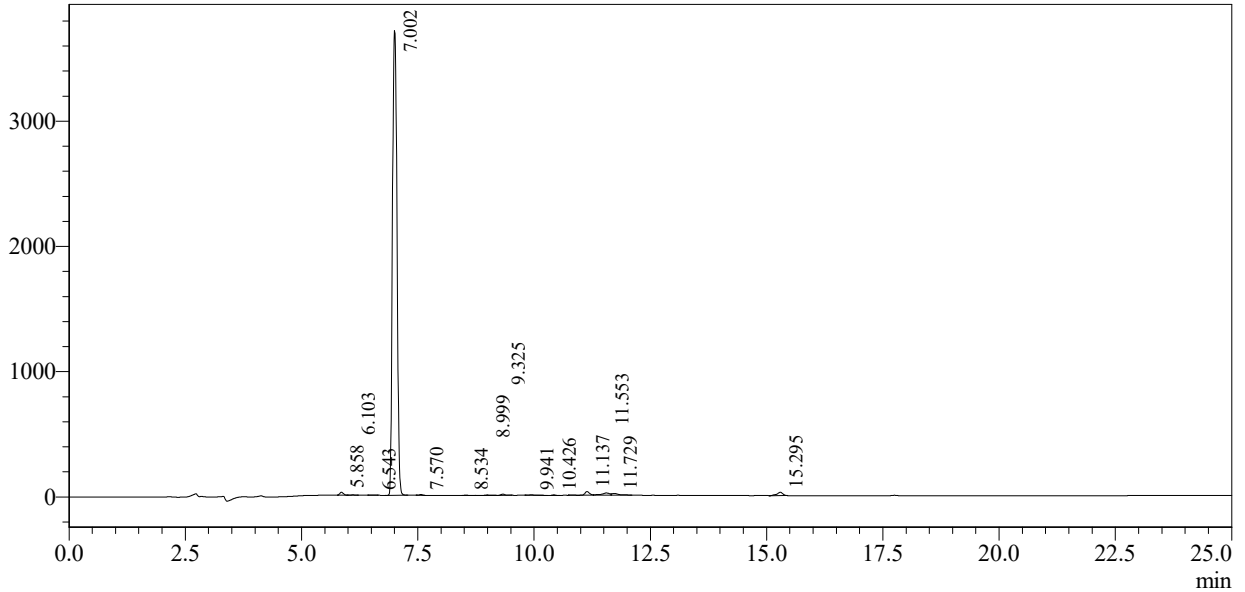

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.858	117110	22652	0.449
2	6.103	13298	2847	0.051
3	6.543	4243	807	0.016
4	7.002	24969948	3708685	95.806
5	7.570	25030	5935	0.096
6	8.534	10860	2292	0.042
7	8.999	27031	3603	0.104
8	9.325	63076	10265	0.242
9	9.941	30326	3367	0.116
10	10.426	17406	4090	0.067
11	11.137	207415	29111	0.796
12	11.553	215413	16986	0.827
13	11.729	129777	13323	0.498
14	15.295	232036	26356	0.890
Total		26062970	3850322	100.000