

Sample Name : Calcitonin Gene Related Peptide (CGRP) II, rat  
 Cat No. : RP11092  
 Lot No. : E7013319J  
 Time Processed : 8:39:45 AM  
 Month-Day-Year Processed : 10/15/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>  
 Column : Alltima™ C18 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

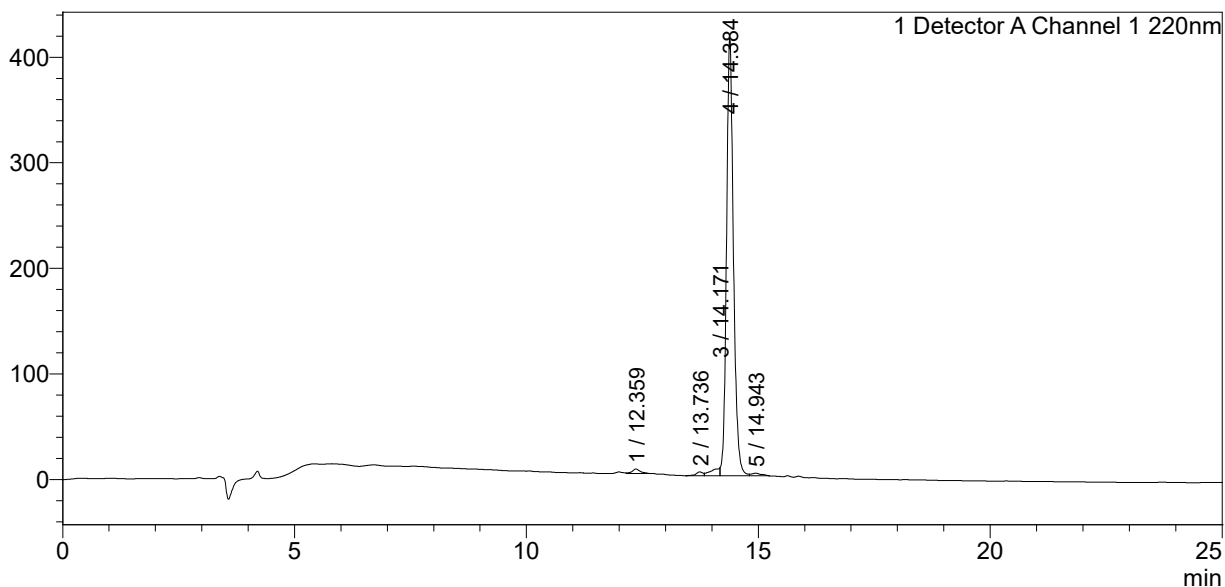

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.359	56076	4431	1.239
2	13.736	36294	3585	0.802
3	14.171	97648	7120	2.157
4	14.384	4302017	414694	95.015
5	14.943	35668	2390	0.788
Total		4527703	432220	100.000