

Sample Name: Dermorphin
 Cat No. : RP10427
 Lot No. : E6990019J
 Time Processed: 4:03:34 AM
 Month-Day-Year Processed :10/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010325

<Chromatogram>

mV

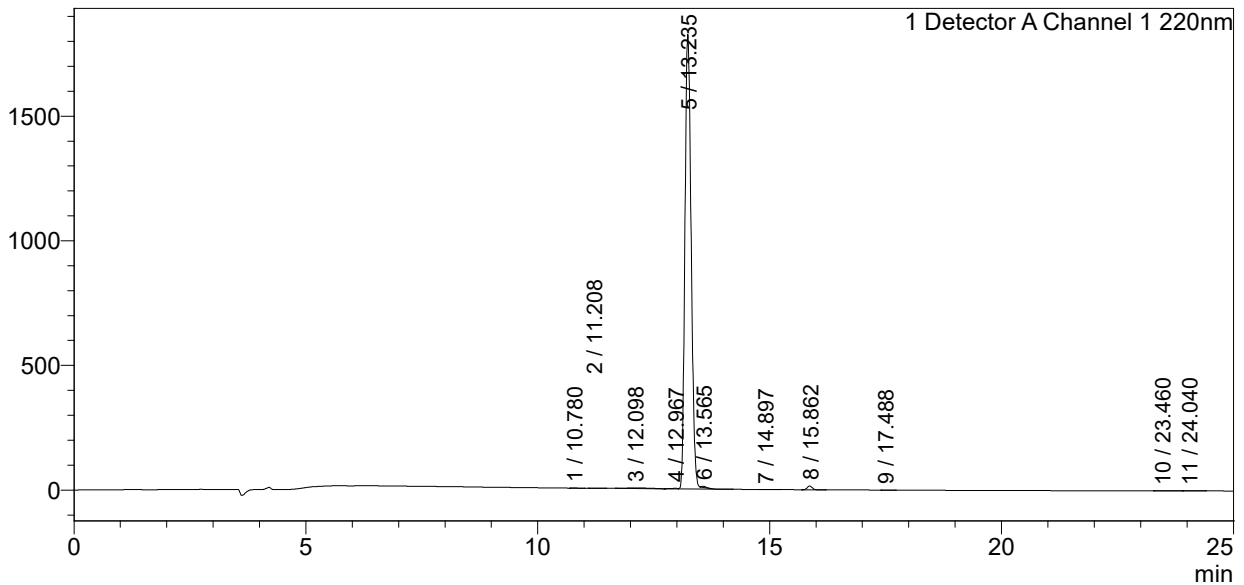

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.780	7828	1437	0.045
2	11.208	1088	89	0.006
3	12.098	77522	2180	0.446
4	12.967	19857	2154	0.114
5	13.235	17109699	1824423	98.520
6	13.565	27247	4345	0.157
7	14.897	3534	278	0.020
8	15.862	114961	15579	0.662
9	17.488	1366	168	0.008
10	23.460	2157	139	0.012
11	24.040	1394	81	0.008
Total		17366652	1850874	100.000