


Mass Spectrum

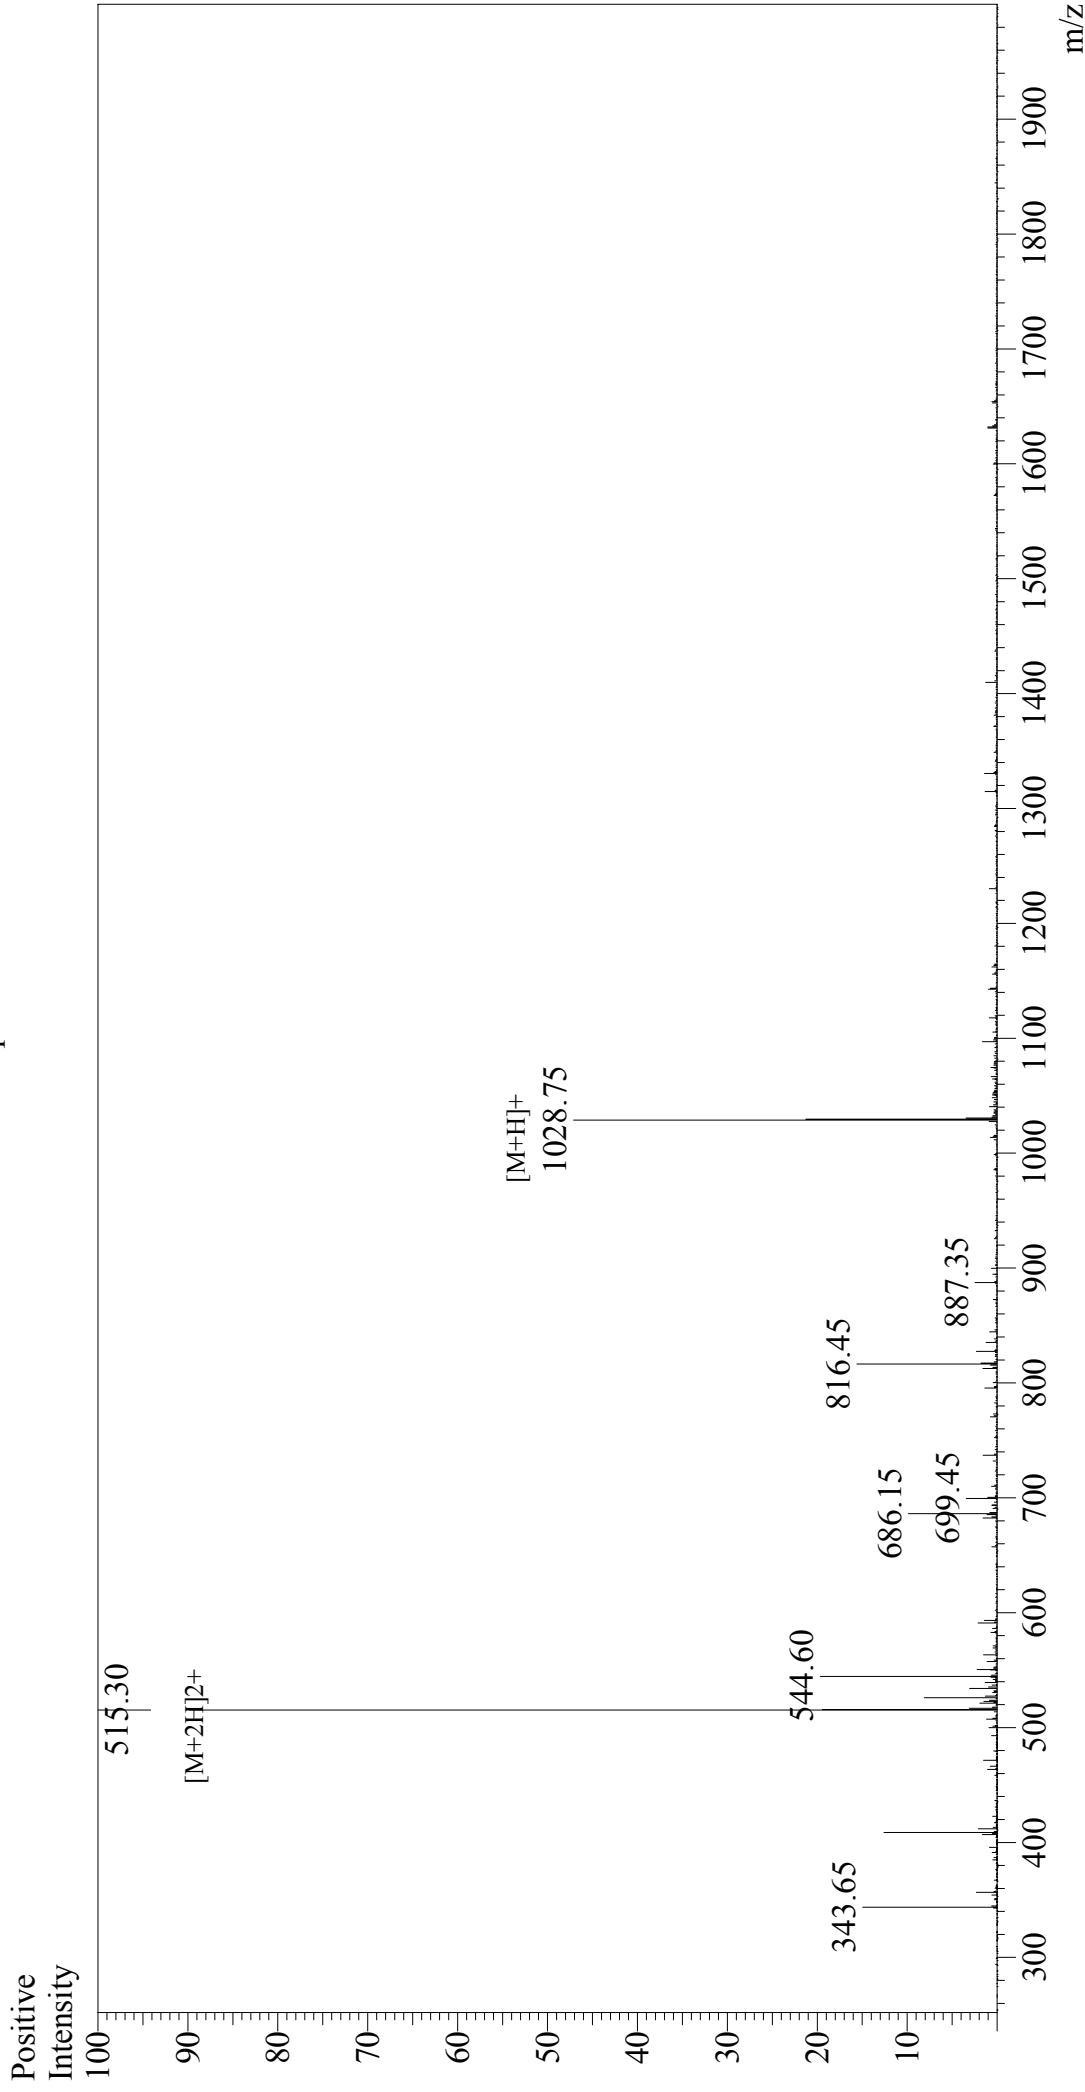

Sample Information

Acquired by : Gary
Month-Day Processed : 06/02/17
Time Processed : 15:12:10
Injection Volume : 0.2
Sample Name : p5 Ligand for Dnak and D naJ
Cat No. : RP20327
Lot No. : PE0271706
Theoretical MW : 1028.30
Observed MW : 1028.60

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH