

Sample Name :HEX3
 Cat No. :RP20346
 Lot No. :E4942819I
 Time Processed :10:18:45
 Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

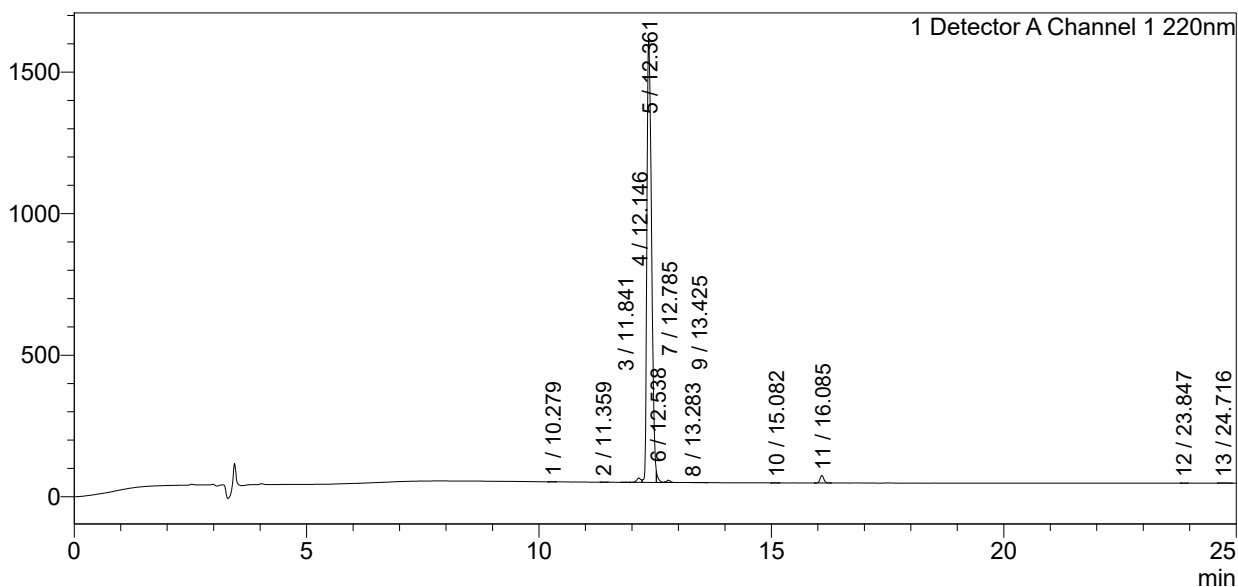

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.279	1471	305	0.013
2	11.359	1276	321	0.011
3	11.841	3931	821	0.035
4	12.146	99068	15330	0.870
5	12.361	10984782	1567881	96.436
6	12.538	95517	30439	0.839
7	12.785	39362	7392	0.346
8	13.283	3197	350	0.028
9	13.425	3859	511	0.034
10	15.082	1859	278	0.016
11	16.085	150244	26531	1.319
12	23.847	1257	244	0.011
13	24.716	4969	637	0.044
Total		11390789	1651040	100.000