


Mass Spectrum

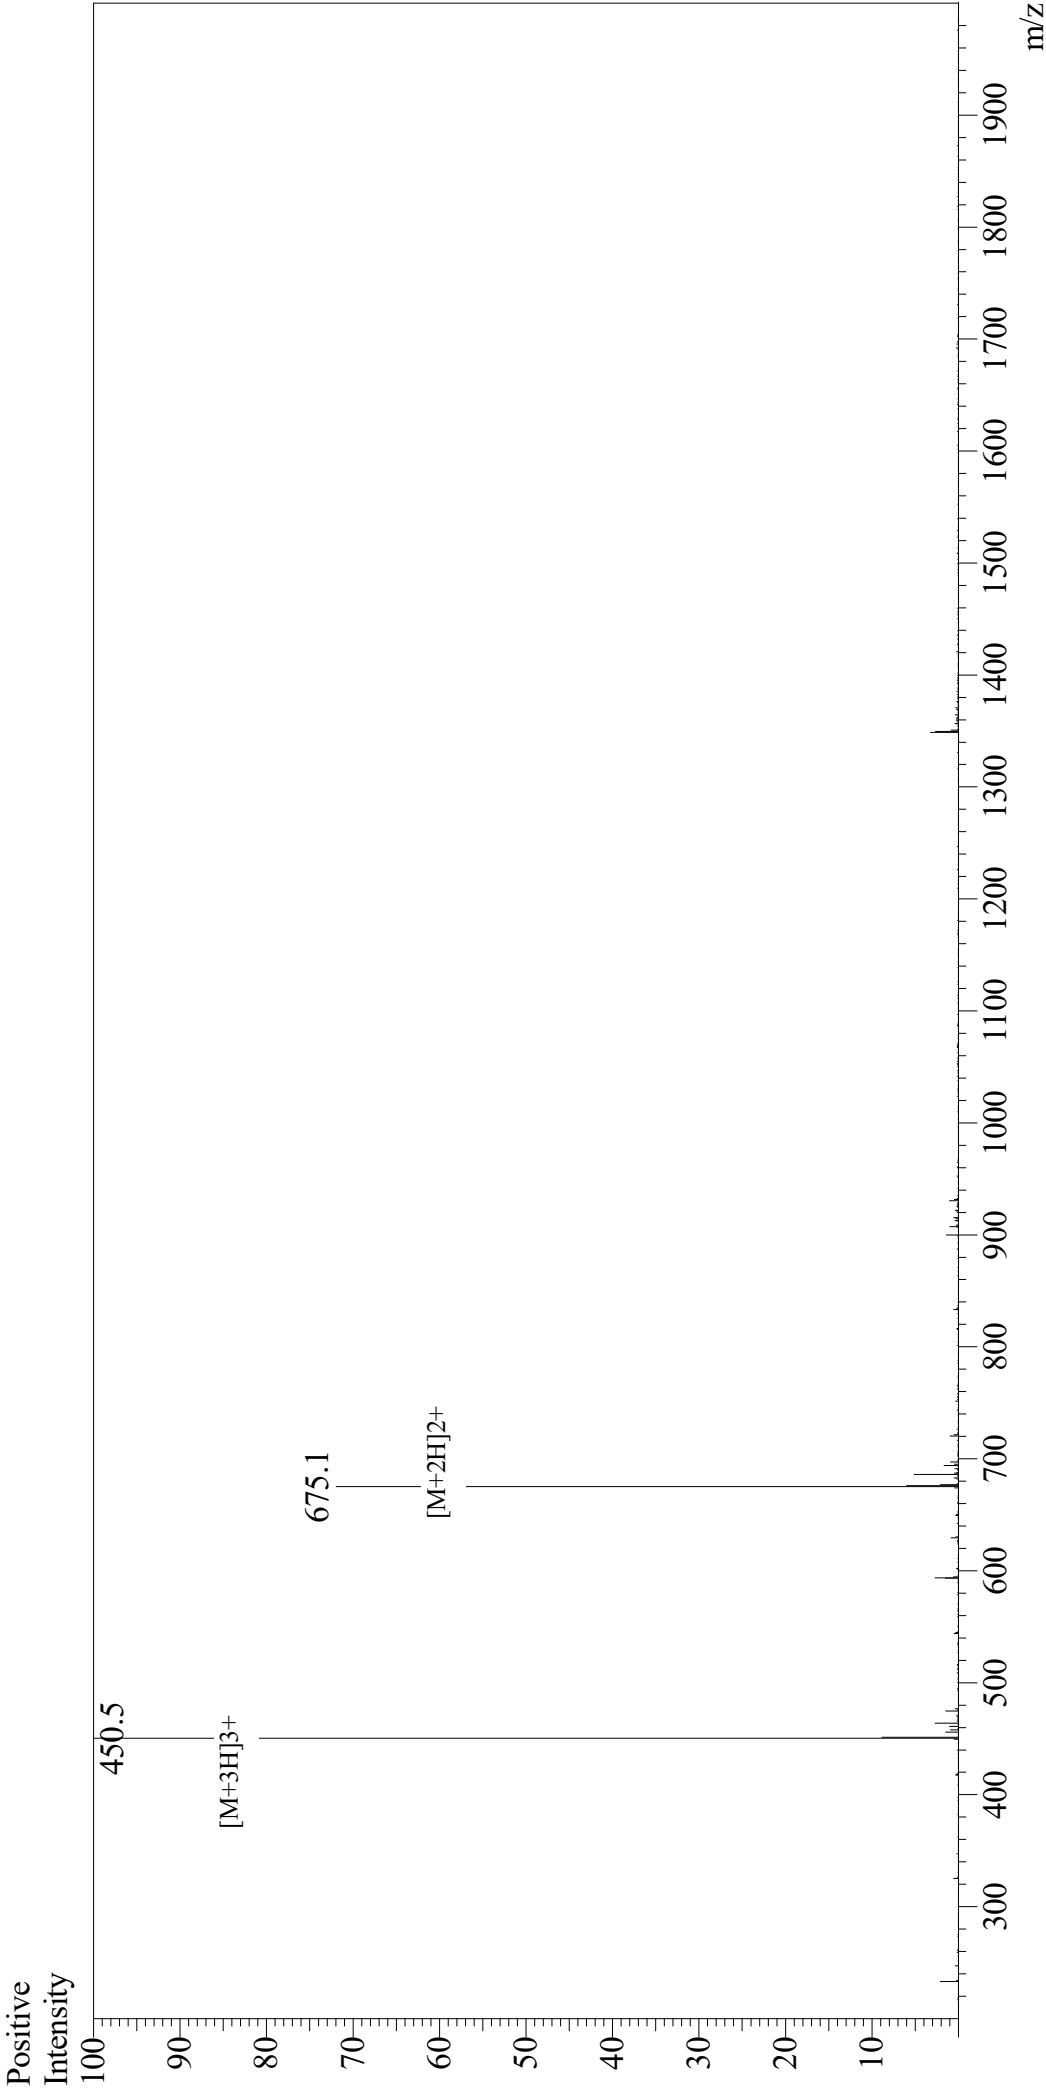

Sample Information

User : Gary
Month-Day Processed : 01/07/20
Time Processed : 05:11:23 PM
Injection Volume : 0.3
Sample Name : BDC2.5 mimotope 1040-31
Cat No. : RP20518
Lot No. : E7372120A
Theoretical MW : 1348.60
Observed MW : 1348.5

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH