

Sample Name : β -Amyloid (1-42), rat
 Cat No. :RP10013
 Lot No. :E3605820C
 Time Processed :15:15:58
 Month-Day-Year Processed :04/15/2020

Pump A : 0.5% Ammonia solution in 100% water (v/v)
 Pump B : 0.2% Ammonia solution in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : UniPS 10-300 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

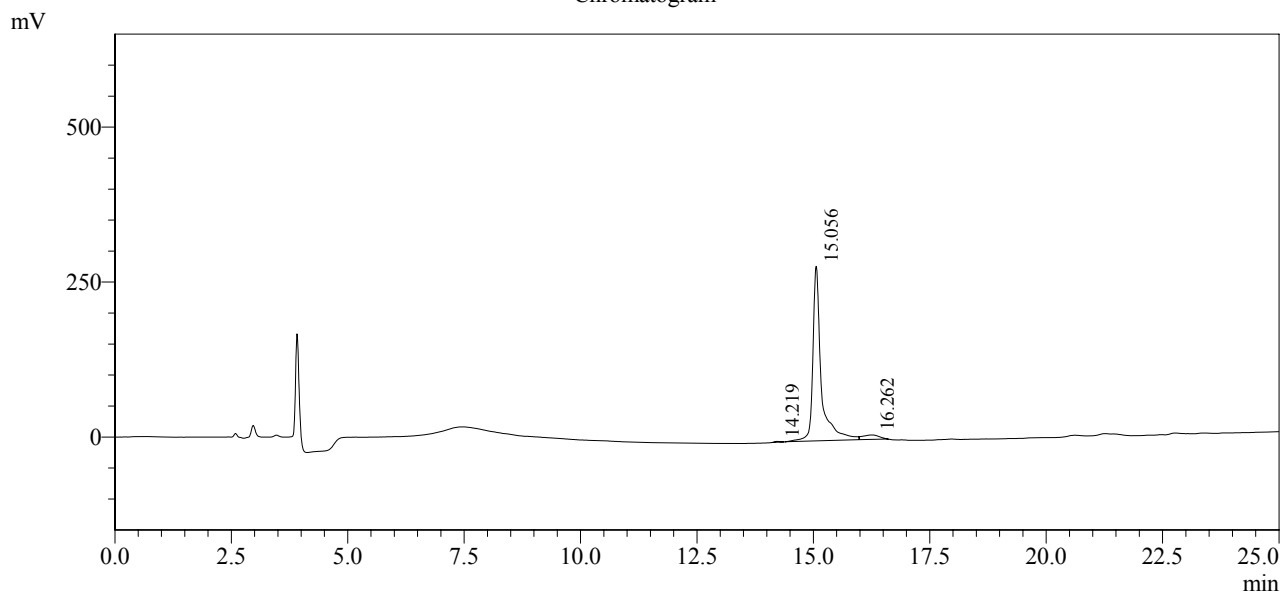

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.219	10220	1361	0.272
2	15.056	3574228	281773	95.032
3	16.262	176614	7142	4.696
Total		3761063	290275	100.000