

Sample Name :N-Acetyl- α -Endorphin
 Cat No. : RP11333
 Lot No. : E1588621G
 Time Processed : 2:34:00
 Month-Day-Year Processed : 07/13/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

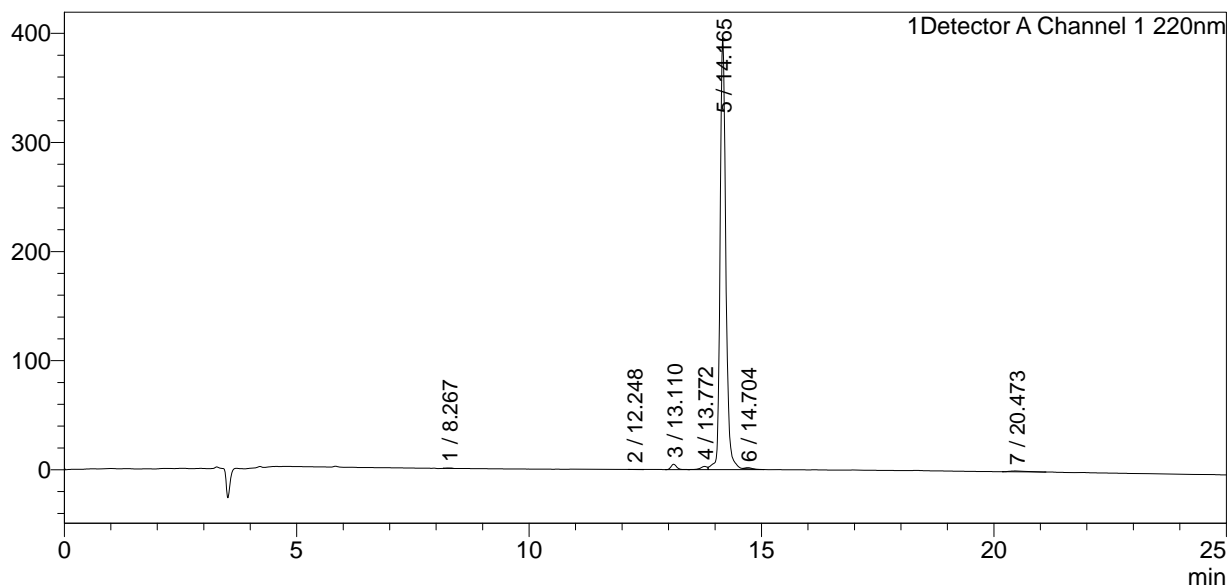

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.267	3599	545	0.103
2	12.248	2176	292	0.062
3	13.110	42002	4922	1.198
4	13.772	29854	2929	0.852
5	14.165	3399081	394048	96.958
6	14.704	8992	1016	0.256
7	20.473	20007	812	0.571
Total		3505711	404563	100.000