

Sample Name :Bradykinin  
 Cat No: PR11129  
 Lot No: E7998720L  
 Time Processed :23:47:01  
 Month-Day-Year Processed :12/29/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ20010139

### <Chromatogram>

mV

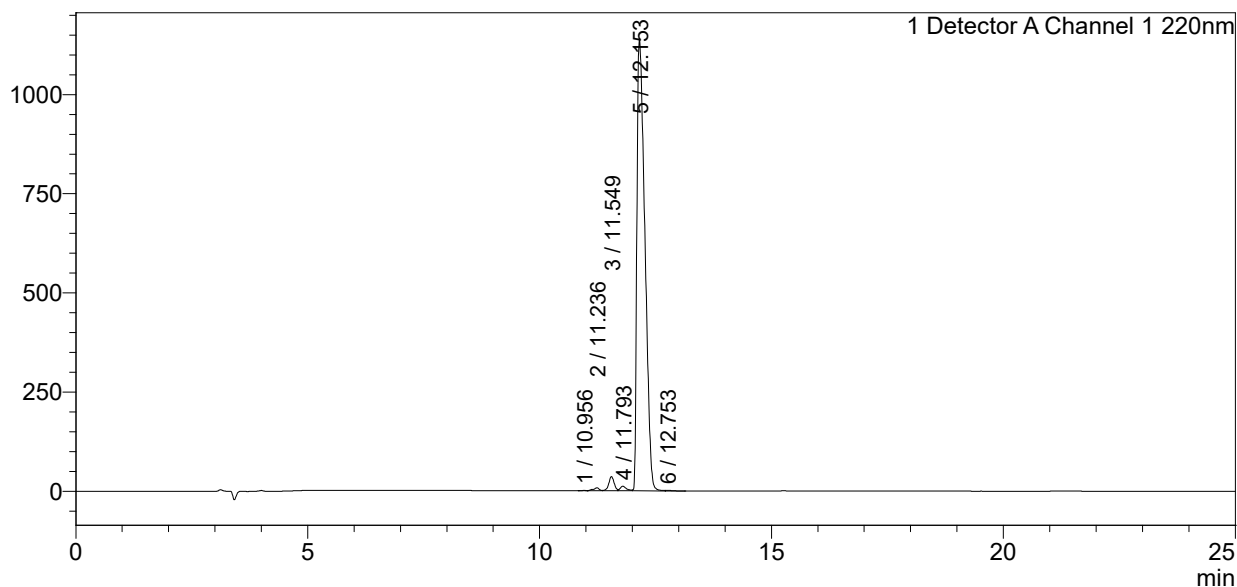

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.956	4741	688	0.034
2	11.236	69290	7682	0.491
3	11.549	290812	36071	2.060
4	11.793	109598	11934	0.777
5	12.153	13626725	1140075	96.548
6	12.753	12744	1373	0.090
Total		14113911	1197824	100.000