

Sample Name :HPV16 E7(86-93)
 Cat. No. :RP20499 Lot. No. :PE2111711
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

<Chromatogram>

mV

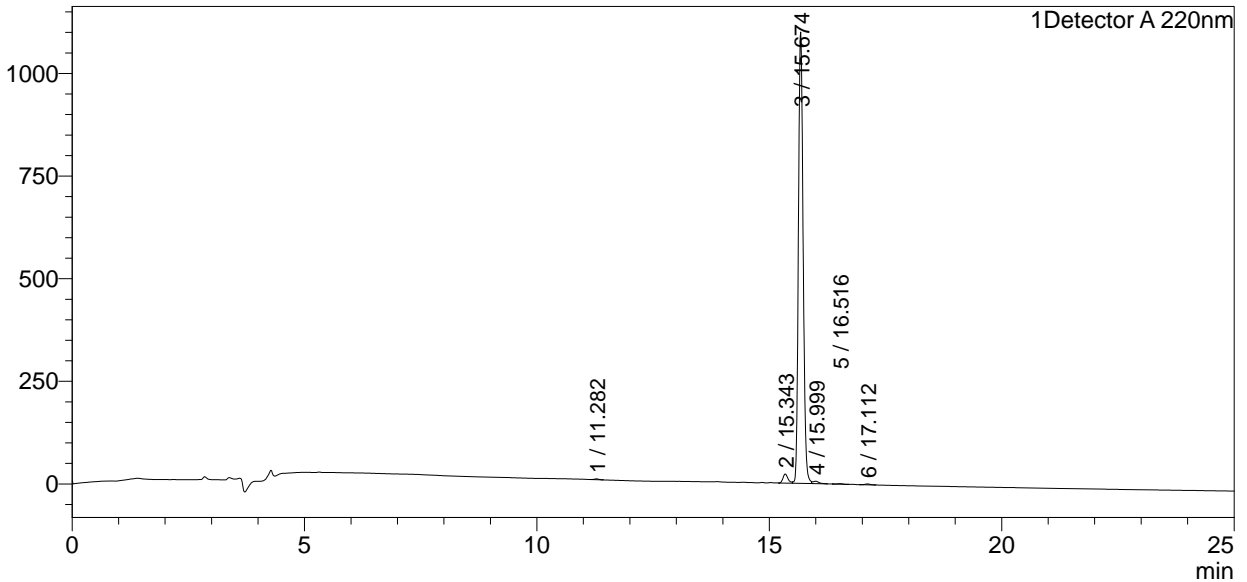

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.282	11659	2007	0.146
2	15.343	166626	22225	2.091
3	15.674	7710774	1099440	96.766
4	15.999	52429	5858	0.658
5	16.516	10712	1440	0.134
6	17.112	16312	2163	0.205
Total		7968512	1133132	100.000