

Sample Name :Hexa-His
 Cat No. :RP11737
 Lot No. :E3601621E
 Time Processed : 11:10:16 AM
 Month-Day-Year Processed : 05/15/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

mV

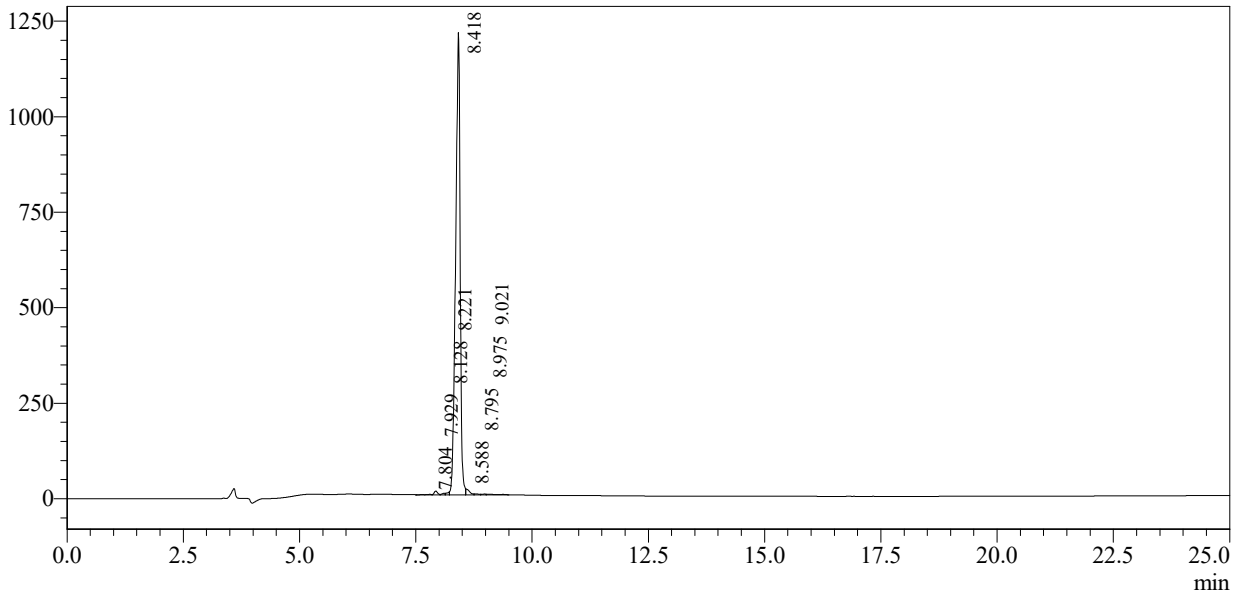

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.804	5099	985	0.061
2	7.929	47693	10044	0.568
3	8.128	19450	4149	0.231
4	8.221	29264	7057	0.348
5	8.418	8172214	1209698	97.242
6	8.588	79025	14674	0.940
7	8.795	15861	2098	0.189
8	8.975	11462	1768	0.136
9	9.021	23945	1700	0.285
Total		8404012	1252173	100.000