

Sample Name :Angiotensin II, human
 Cat No. :RP11257
 Lot No. :E6077020C
 Time Processed :8:32:24
 Month-Day-Year Processed :03/27/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

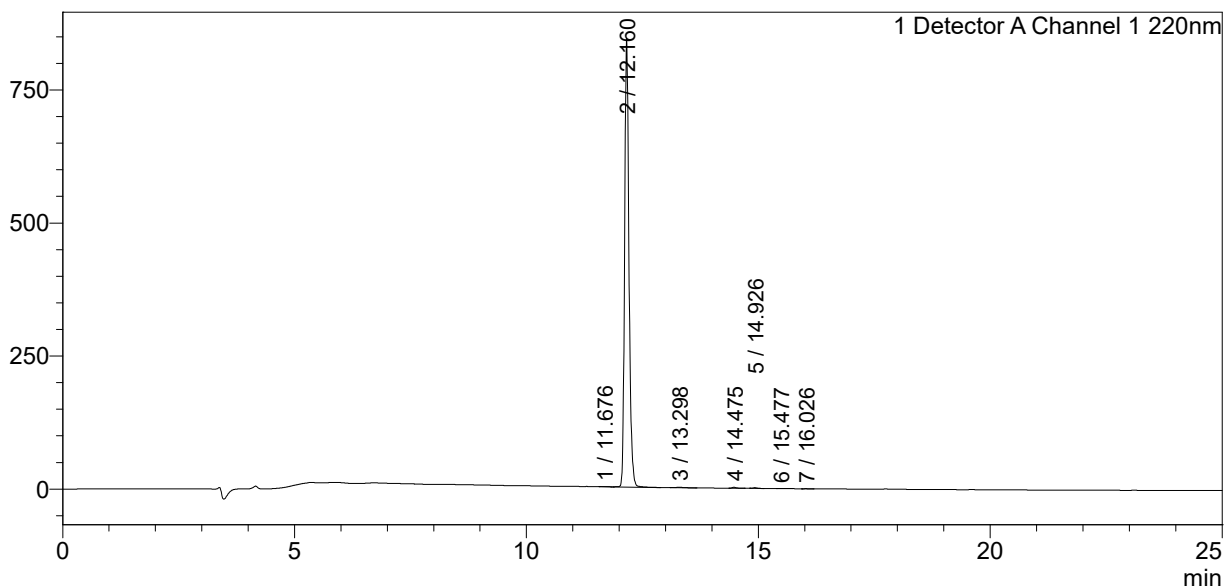

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.676	2964	380	0.053
2	12.160	5531967	843819	99.425
3	13.298	8604	800	0.155
4	14.475	10417	1652	0.187
5	14.926	7680	1228	0.138
6	15.477	1011	92	0.018
7	16.026	1291	183	0.023
Total		5563934	848154	100.000