

Sample Name :Cecropin B  
 Cat. No. : RP11225  
 Lot. No. : E7291119H  
 Time Processed :8:14:40  
 Month-Day-Year Processed : 09/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

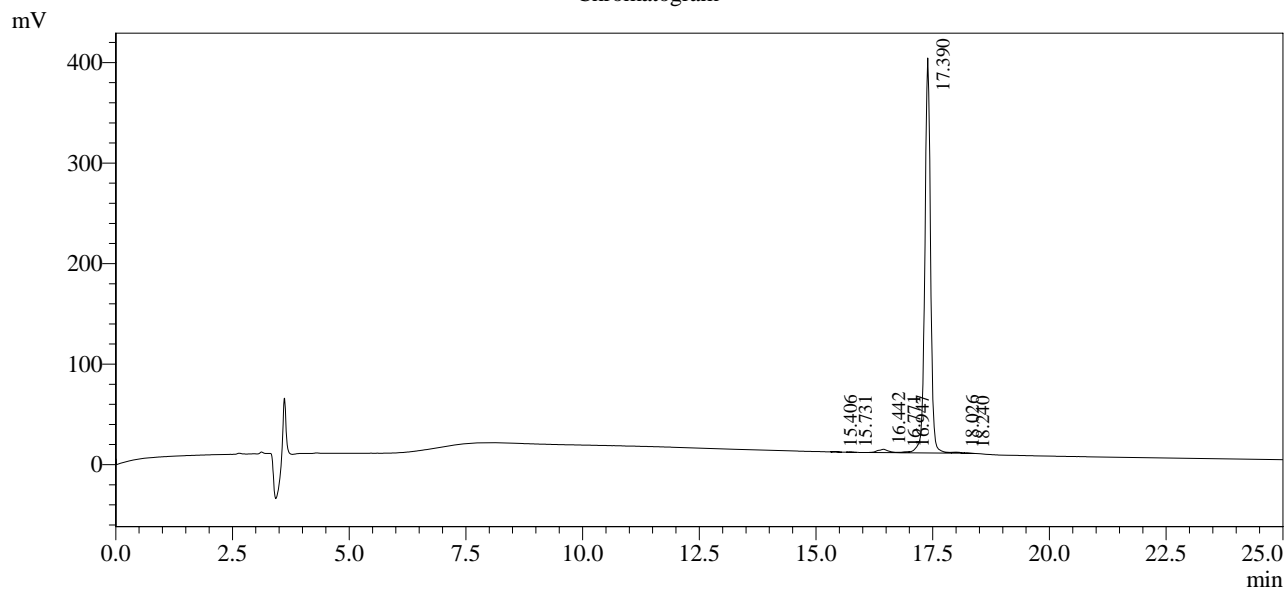

1 Det.A Ch1 / 220nm  
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.406	2369	394	0.069
2	15.731	1701	264	0.050
3	16.442	52352	3326	1.527
4	16.771	3596	578	0.105
5	16.947	9747	1055	0.284
6	17.390	3346538	392932	97.634
7	18.026	9841	1069	0.287
8	18.240	1509	231	0.044
Total		3427652	399848	100.000