

Sample Name : Arg-Gly-Asp-Ser
 Cat. No. : RP10861
 Lot. No. : PE8861901
 Time Processed : 19:38:57
 Month-Day-Year Processed : 01/23/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	0	
5.00	Pumps	Pump B Conc.	0	
20.00	Pumps	Pump B Conc.	30	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	0	
40.00	Pumps	Pump B Conc.	0	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

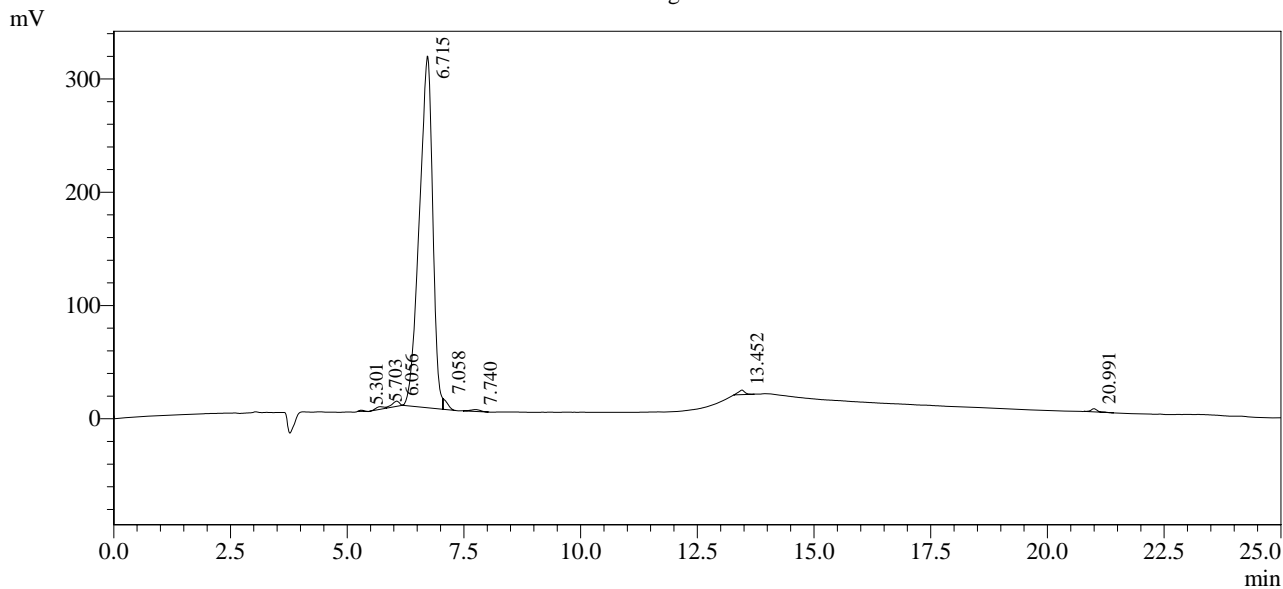

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.301	7459	1117	0.116
2	5.703	28159	2306	0.440
3	6.056	50679	4631	0.791
4	6.715	6167293	310494	96.291
5	7.058	61146	9326	0.955
6	7.740	23582	1611	0.368
7	13.452	38116	4013	0.595
8	20.991	28419	2855	0.444
Total		6404854	336353	100.000