

Sample Name :BNP(1-45), mouse
 Cat No. :RP20365
 Lot No. :E5084620J
 Time Processed :6:41:04
 Month-Day-Year Processed :10/13/20

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

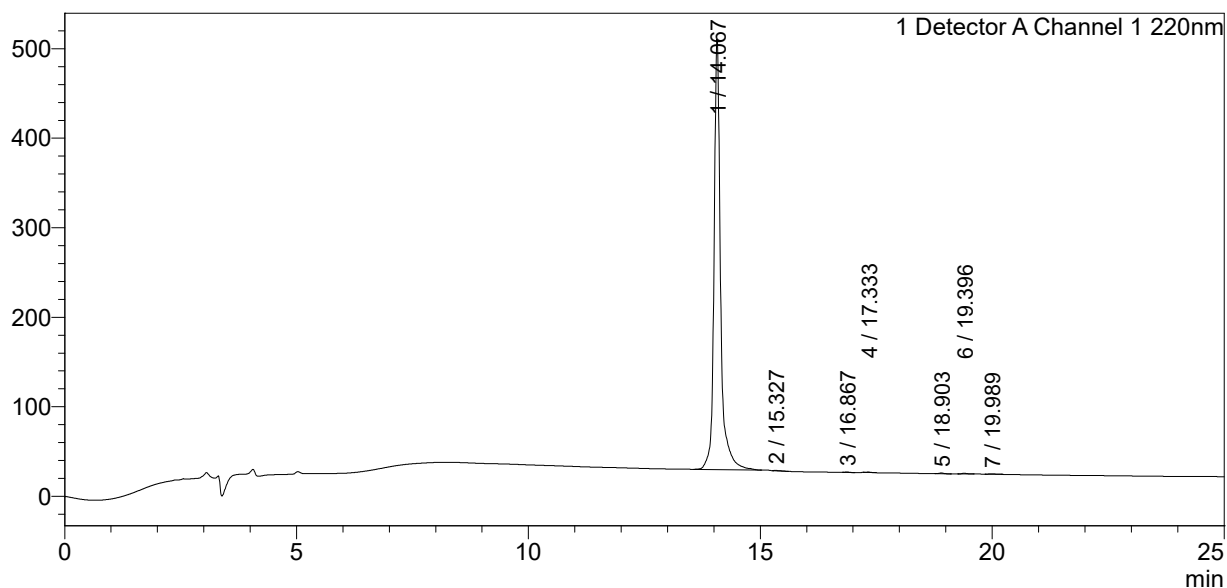

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.067	4743667	481000	99.405
2	15.327	4131	510	0.087
3	16.867	3185	603	0.067
4	17.333	3849	552	0.081
5	18.903	6235	823	0.131
6	19.396	6373	769	0.134
7	19.989	4607	536	0.097
Total		4772047	484793	100.000