

Sample Name : N-Cbz-Phe-Arg-AMC
 Cat. No. : RP11385
 Lot. No. : E47449191
 Time Processed : 5:29:03
 Month-Day-Year Processed : 09/28/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
10.00	Pumps	Pump B Conc.	35	
35.00	Pumps	Pump B Conc.	95	
41.00	Pumps	Pump B Conc.	95	
41.01	Pumps	Pump B Conc.	5	
50.00	Pumps	Pump B Conc.	5	
50.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

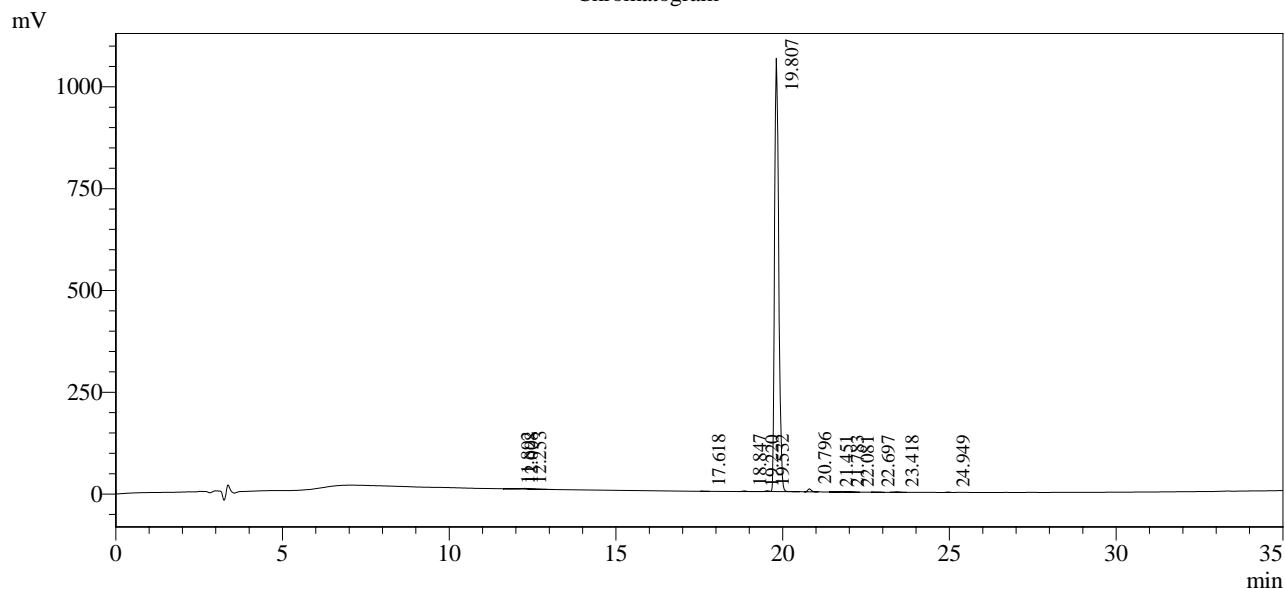

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.892	6426	585	0.068
2	12.008	8427	766	0.090
3	12.253	34536	1979	0.367
4	17.618	1141	127	0.012
5	18.847	10955	1533	0.116
6	19.220	1667	213	0.018
7	19.532	15777	1985	0.168
8	19.807	9251514	1064334	98.373
9	20.796	54572	7274	0.580
10	21.451	1073	133	0.011
11	21.783	3839	458	0.041
12	22.081	1049	152	0.011
13	22.697	1077	49	0.011
14	23.418	10501	984	0.112
15	24.949	1990	358	0.021
Total		9404542	1080929	100.000