

Sample Name :Gly-Arg-Gly-Asp-Ser
Cat No. : RP10848
Lot No. : E5820620B
Time Processed :12:50:32
Month-Day-Year Processed :02/16/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
5.00	Pumps	Solvent B Conc.	0
20.00	Pumps	Solvent B Conc.	30
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	0
35.00	Pumps	Solvent B Conc.	0
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
Equipment:ZJ19010141

<Chromatogram>

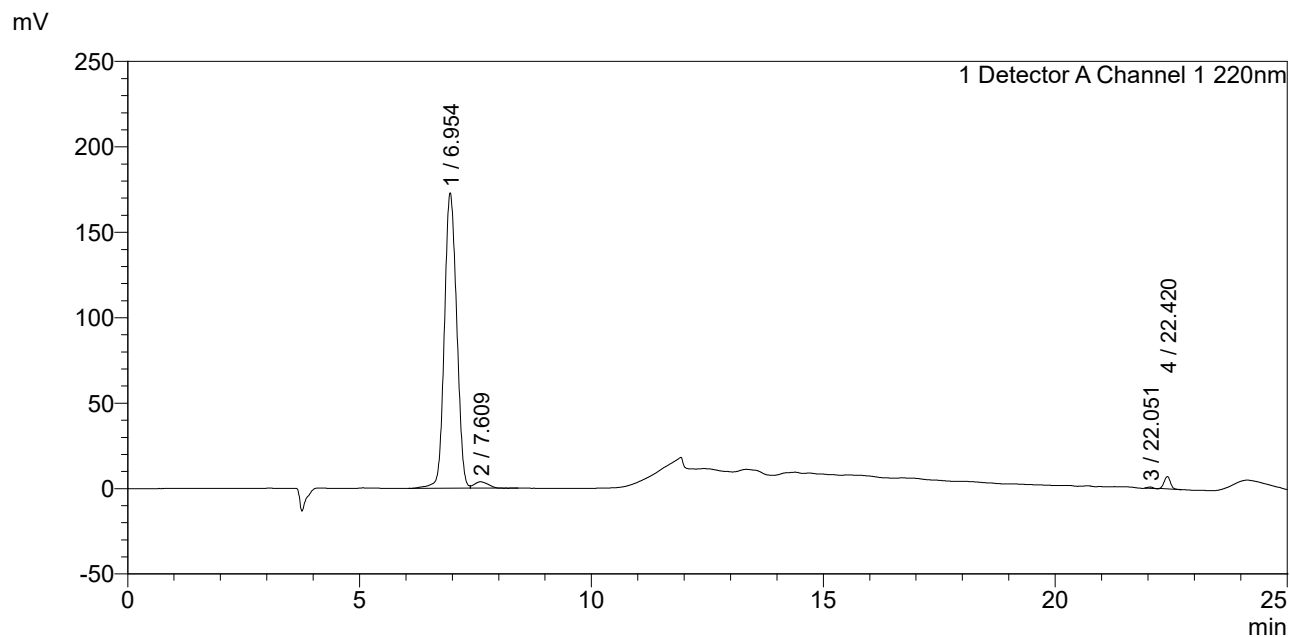

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.954	3194958	172960	95.541
2	7.609	77071	3768	2.305
3	22.051	6231	833	0.186
4	22.420	65804	7203	1.968
Total		3344064	184764	100.000