

Sample Name : Gastrin-1, human
 Cat. No. :RP12740
 Lot. No. :PE8301807

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
10.00	Pumps	Pump A B.Conc	35	
35.00	Pumps	Pump A B.Conc	95	
41.00	Pumps	Pump A B.Conc	95	
41.01	Pumps	Pump A B.Conc	5	
50.00	Pumps	Pump A B.Conc	5	
50.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

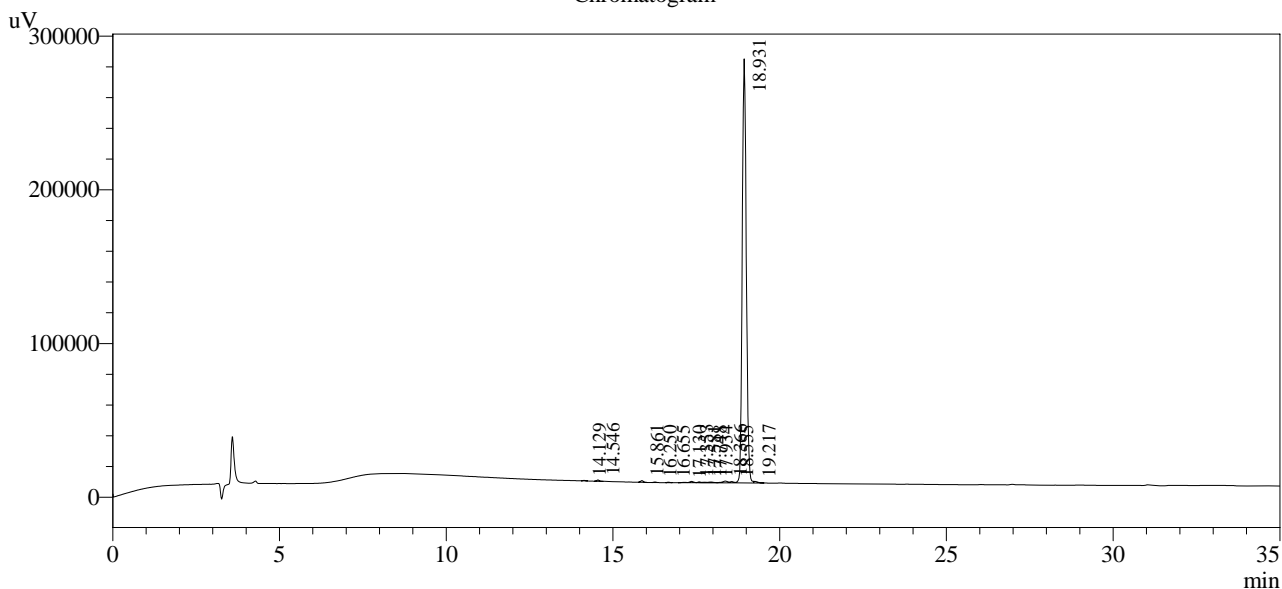

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.129	1623	333	0.068
2	14.546	4719	835	0.197
3	15.861	6321	1116	0.264
4	16.250	1915	357	0.080
5	16.655	1519	295	0.063
6	17.130	2186	248	0.091
7	17.353	6986	826	0.291
8	17.581	3508	555	0.146
9	17.748	4239	365	0.177
10	17.934	4614	536	0.192
11	18.366	13755	1117	0.573
12	18.555	7034	836	0.293
13	18.931	2332160	275936	97.228
14	19.217	8069	1052	0.336
Total		2398649	284405	100.000