

Sample Name :W Peptide, WKYVMm  
 Cat No. :RP20299  
 Lot No. :E1524720F  
 Time Processed :7:23:16  
 Month-Day-Year Processed :06/11/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010507

<Chromatogram>

mV

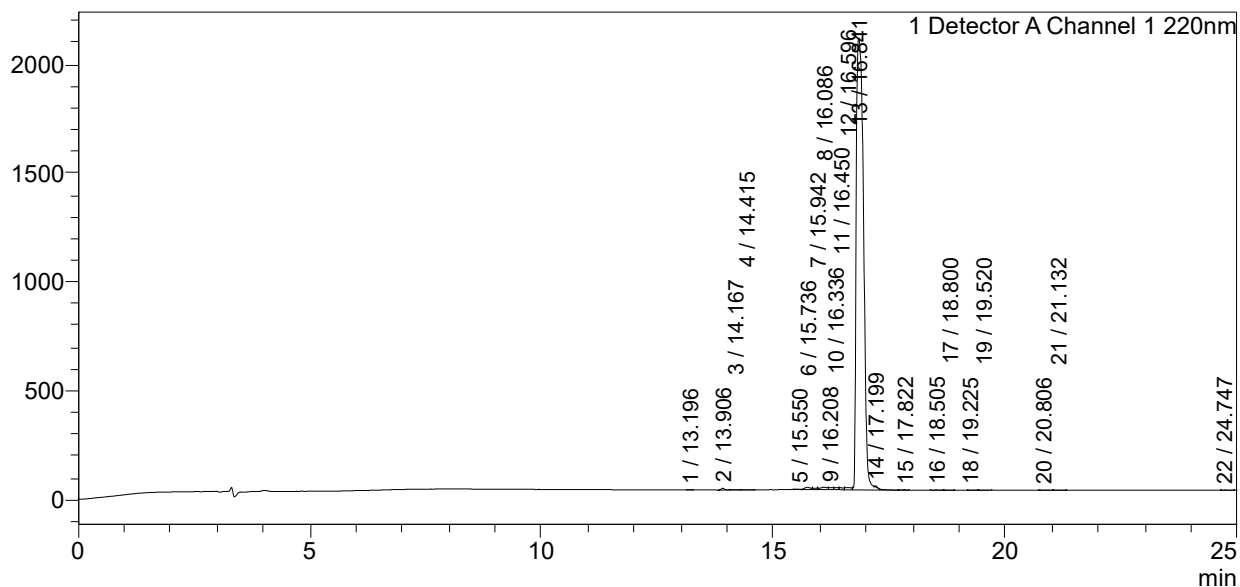

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.196	2795	641	0.012
2	13.906	43318	8576	0.187
3	14.167	4305	488	0.019
4	14.415	6050	585	0.026
5	15.550	4420	655	0.019
6	15.736	95421	9807	0.412
7	15.942	51517	6612	0.223
8	16.086	97143	11235	0.420
9	16.208	64343	9462	0.278
10	16.336	72589	9417	0.314
11	16.450	52523	9029	0.227
12	16.596	105954	9879	0.458
13	16.841	22474723	2077877	97.142
14	17.199	16446	4428	0.071
15	17.822	12003	2034	0.052

Peak#	Ret. Time	Area	Height	Area%
16	18.505	8729	1168	0.038
17	18.800	4275	499	0.018
18	19.225	1666	219	0.007
19	19.520	3259	387	0.014
20	20.806	2018	332	0.009
21	21.132	4751	663	0.021
22	24.747	7602	1035	0.033
Total		23135849	2165028	100.000