

Sample Name : DYKDDDDK Peptide  
 Cat. No. : RP10586  
 Lot. No. : PE3091702

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	0	
5.00	Pumps	Pump A B.Conc	0	
20.00	Pumps	Pump A B.Conc	30	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	0	
40.00	Pumps	Pump A B.Conc	0	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : UniPS 10-300 10µm 4.6 x 250 mm

Chromatogram

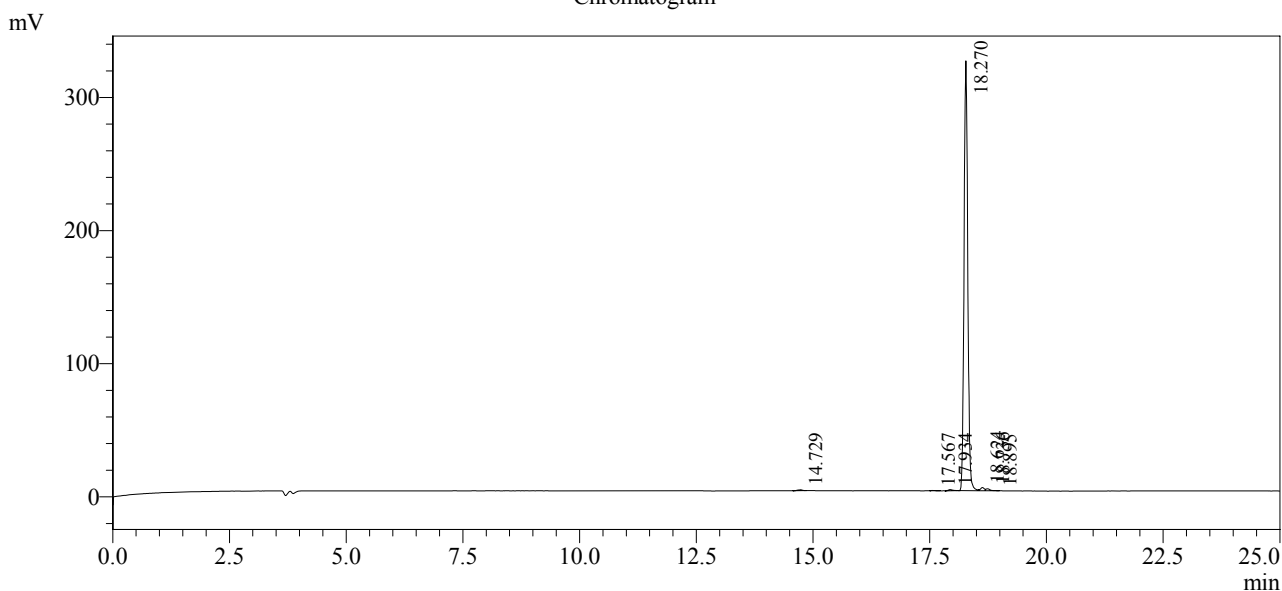

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.729	4243	609	0.233
2	17.567	1292	254	0.071
3	17.934	5519	865	0.303
4	18.270	1787916	322907	98.149
5	18.624	13574	2383	0.745
6	18.736	8607	1480	0.473
7	18.895	477	137	0.026
Total		1821628	328635	100.000