

Sample Name :OVA Peptide (257-264)
 Cat No. :RP10611
 Lot No. :E6812020H
 Time Processed :17:24:41
 Month-Day-Year Processed :08/06/20

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

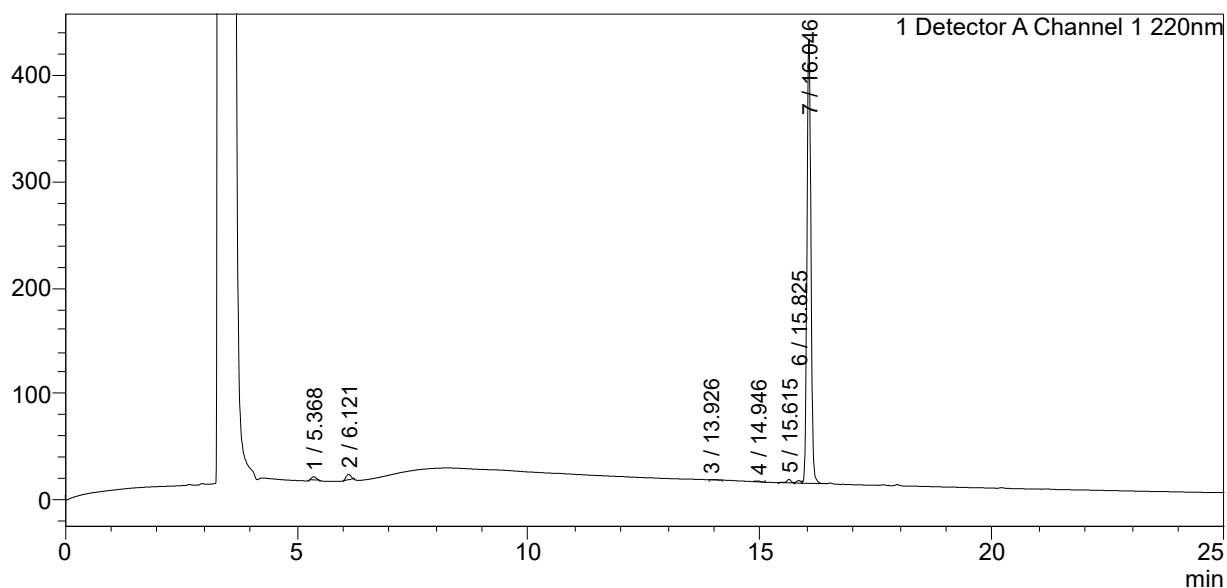

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.368	19656	2842	0.756
2	6.121	35833	4968	1.378
3	13.926	1055	79	0.041
4	14.946	4614	808	0.177
5	15.615	22516	3214	0.866
6	15.825	15854	2405	0.610
7	16.046	2501508	417273	96.174
Total		2601036	431589	100.000