

Sample Name :CREBtide  
Cat. No. : RP10142  
Lot. No.:E6767919H  
Time Processed :14:00:11  
Month-Day-Year Processed :08/29/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
Total Flow:1 ml/min  
Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

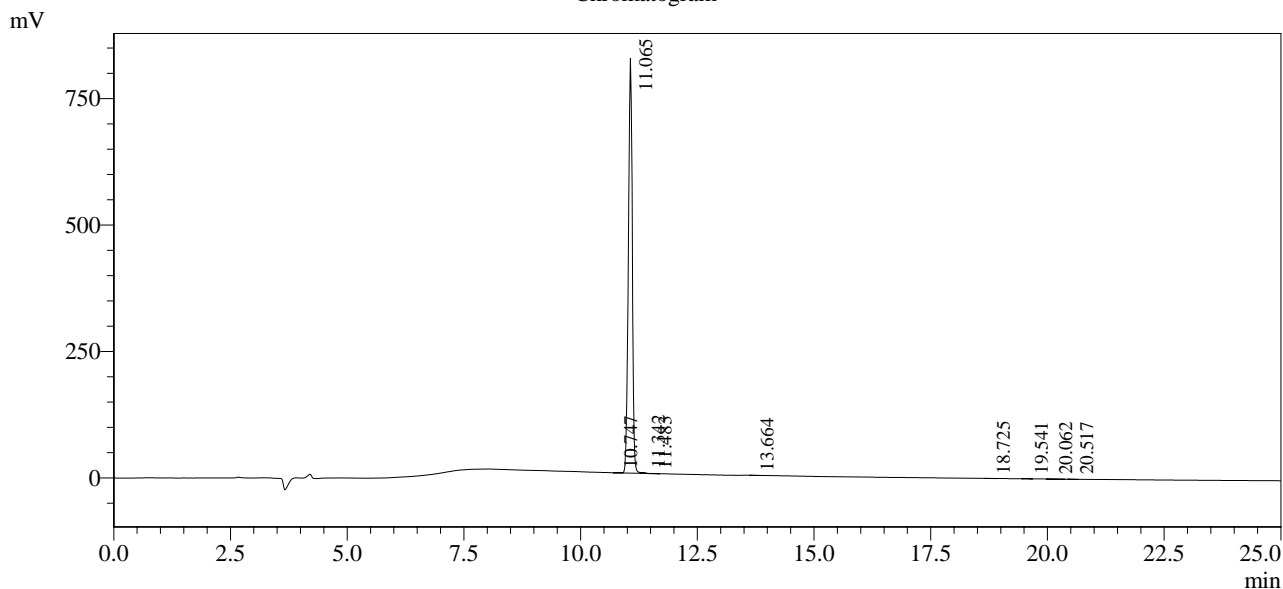

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.747	1295	76	0.027
2	11.065	4821339	820402	99.543
3	11.342	12536	1822	0.259
4	11.483	1441	186	0.030
5	13.664	1404	125	0.029
6	18.725	1052	148	0.022
7	19.541	1925	343	0.040
8	20.062	1274	129	0.026
9	20.517	1221	192	0.025
Total		4843487	823422	100.000