

Sample Name : β -Amyloid Protein Precursor 770 (135-155)
 Cat No.: RP20196
 Lot No.: E1695019J
 Time Processed: 7:16:30
 Month-Day-Year Processed: 10/27/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010014

<Chromatogram>

mV

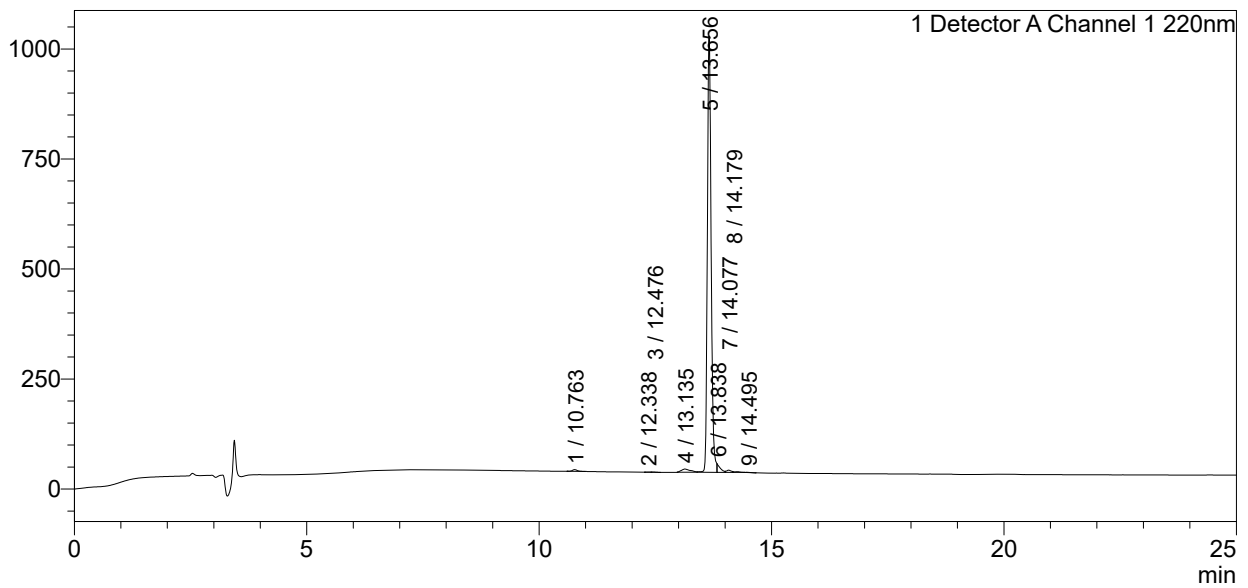

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.763	29651	4066	0.504
2	12.338	1870	377	0.032
3	12.476	2376	429	0.040
4	13.135	100935	7318	1.714
5	13.656	5617716	991198	95.422
6	13.838	86236	18288	1.465
7	14.077	33181	4829	0.564
8	14.179	11403	1472	0.194
9	14.495	3874	813	0.066
Total		5887243	1028790	100.000