

Sample Name :BNP(1-45), mouse
 Cat. No. :RP20365
 Lot. No. : PE2101904
 Time Processed : 16:16:28
 Month-Day-Year Processed : 06/02/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

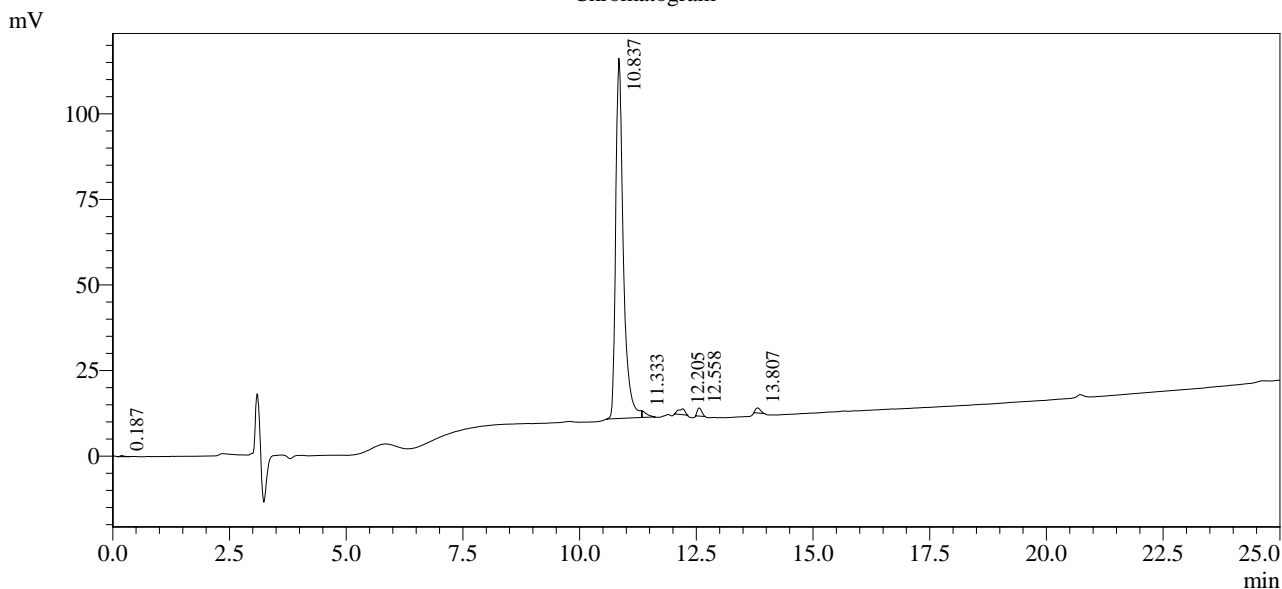

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	0.187	1915	340	0.153
2	10.837	1192646	105210	95.342
3	11.333	12799	1964	1.023
4	12.205	17187	1740	1.374
5	12.558	15536	2363	1.242
6	13.807	10825	1487	0.865
Total		1250907	113103	100.000