

Sample Name :  $\beta$ -Amyloid (1-42), human  
 Cat. No. : RP10017  
 Lot. No. : PE3411712

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	10	
25.00	Pumps	Pump A B.Conc	100	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	10	
40.00	Pumps	Pump A B.Conc	10	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

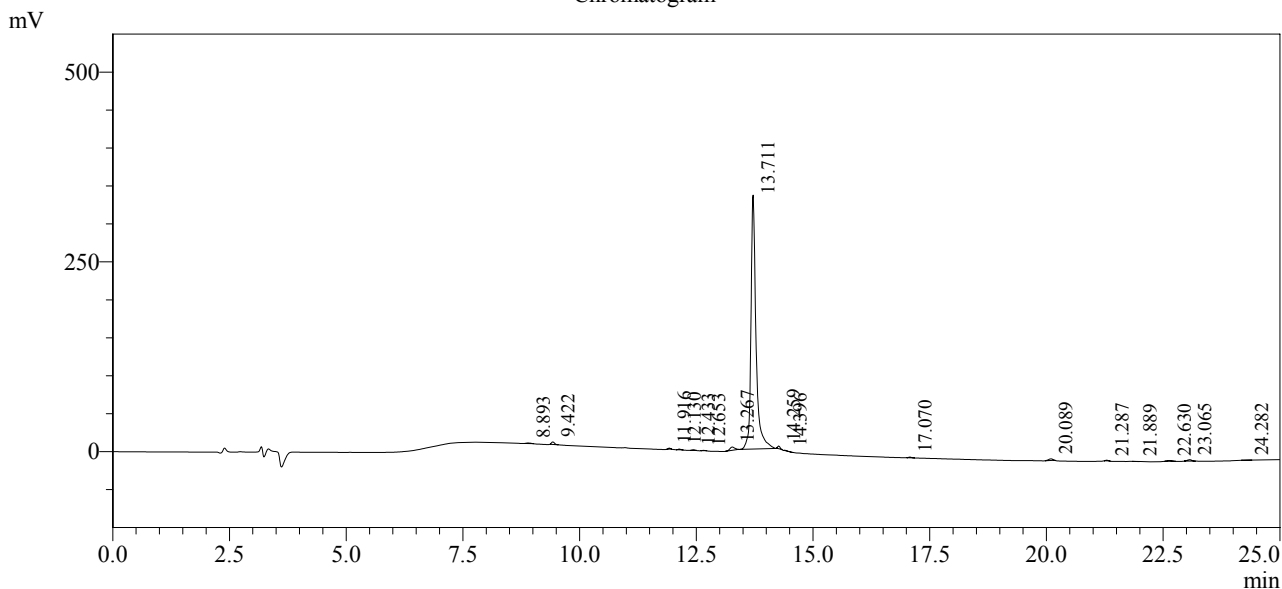

1 Det. A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.893	4105	647	0.155
2	9.422	14366	3300	0.541
3	11.916	4469	1350	0.168
4	12.130	3969	999	0.150
5	12.433	2903	763	0.109
6	12.653	1916	446	0.072
7	13.267	31769	4359	1.197
8	13.711	2531215	334579	95.361
9	14.259	12453	3476	0.469
10	14.396	1753	383	0.066
11	17.070	3966	920	0.149
12	20.089	13939	2185	0.525
13	21.287	3734	910	0.141
14	21.889	1107	249	0.042
15	22.630	7357	1012	0.277
16	23.065	12375	1915	0.466
17	24.282	2953	431	0.111
Total		2654349	357922	100.000