

Sample Name :Hexa-His
 Cat No. : RP11737
 Lot No. :E4728819I
 Time Processed : 2:14:06
 Month-Day-Year Processed : 09/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	0
5.00	Pumps	Pump B Conc.	0
20.00	Pumps	Pump B Conc.	30
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
31.00	Pumps	Pump B Conc.	95
31.01	Pumps	Pump B Conc.	0
40.00	Pumps	Pump B Conc.	0
40.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment:GK12010012

<Chromatogram>

mV

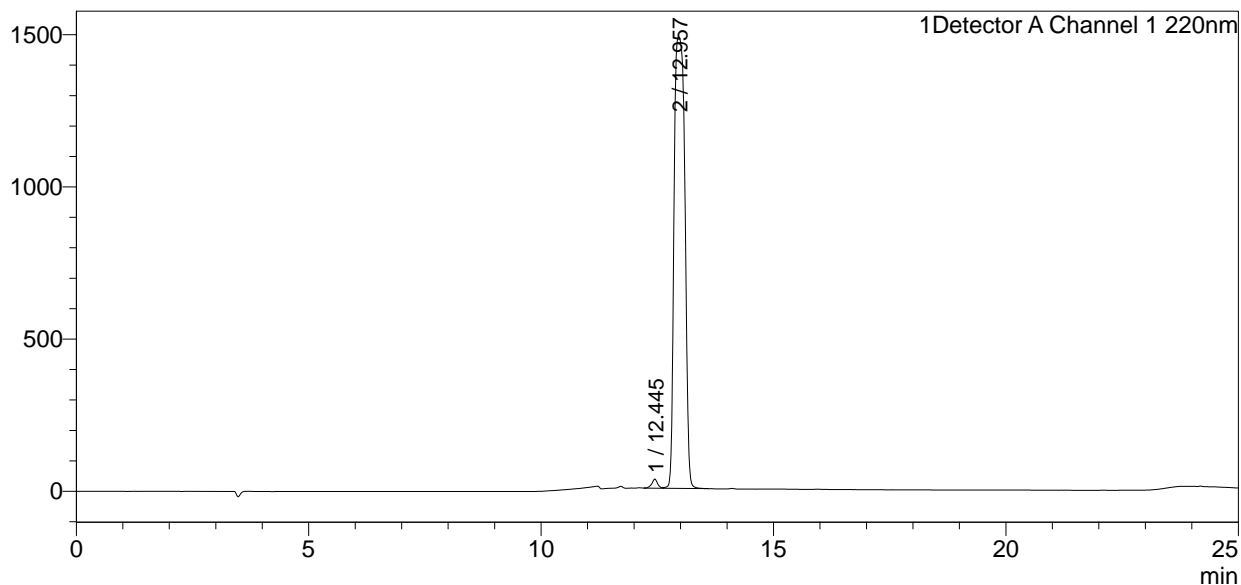

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.445	260386	30234	1.082
2	12.957	23812979	1483601	98.918
Total		24073365	1513836	100.000