

Sample Name :N-Formyl-Nle-Leu-Phe-Nle-Tyr-Lys  
 Cat. No. : RP12959  
 Lot. No. : E4884219I  
 Time Processed :5:06:01  
 Month-Day-Year Processed :09/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

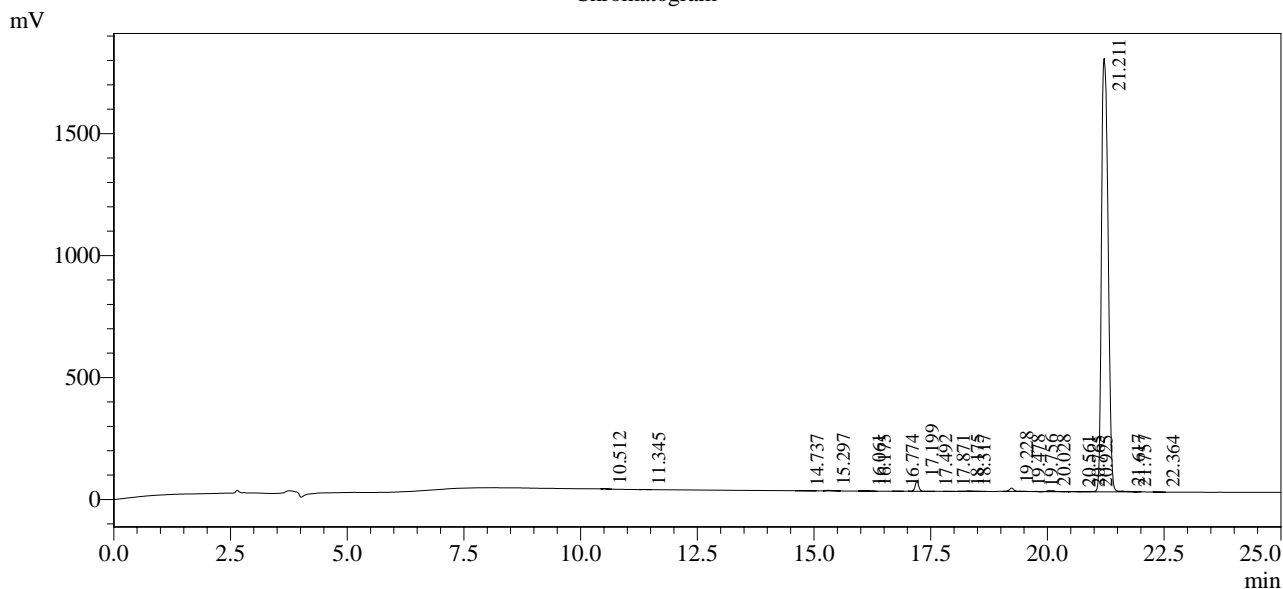

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.512	10139	1977	0.056
2	11.345	4692	858	0.026
3	14.737	6115	811	0.034
4	15.297	21247	2784	0.118
5	16.061	7303	1195	0.040
6	16.175	2757	607	0.015
7	16.774	2451	401	0.014
8	17.199	218622	40543	1.209
9	17.492	3109	275	0.017
10	17.871	2544	430	0.014
11	18.175	3332	524	0.018
12	18.317	20656	2098	0.114
13	19.228	87486	13574	0.484
14	19.478	6147	906	0.034
15	19.756	5448	958	0.030
16	20.028	55158	4374	0.305
17	20.561	8472	1094	0.047
18	20.765	5612	734	0.031
19	20.925	6136	1035	0.034
20	21.211	17593619	1777677	97.315
21	21.617	1208	318	0.007
22	21.757	4180	815	0.023
23	22.364	2681	375	0.015
Total		18079115	1854363	100.000