

Sample Name :  $\beta$ -Amyloid (1-40)  
 Cat. No. : RP10004  
 Lot. No. : PE5021707

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima<sup>TM</sup> C18 4.6 x 250 mm

Chromatogram

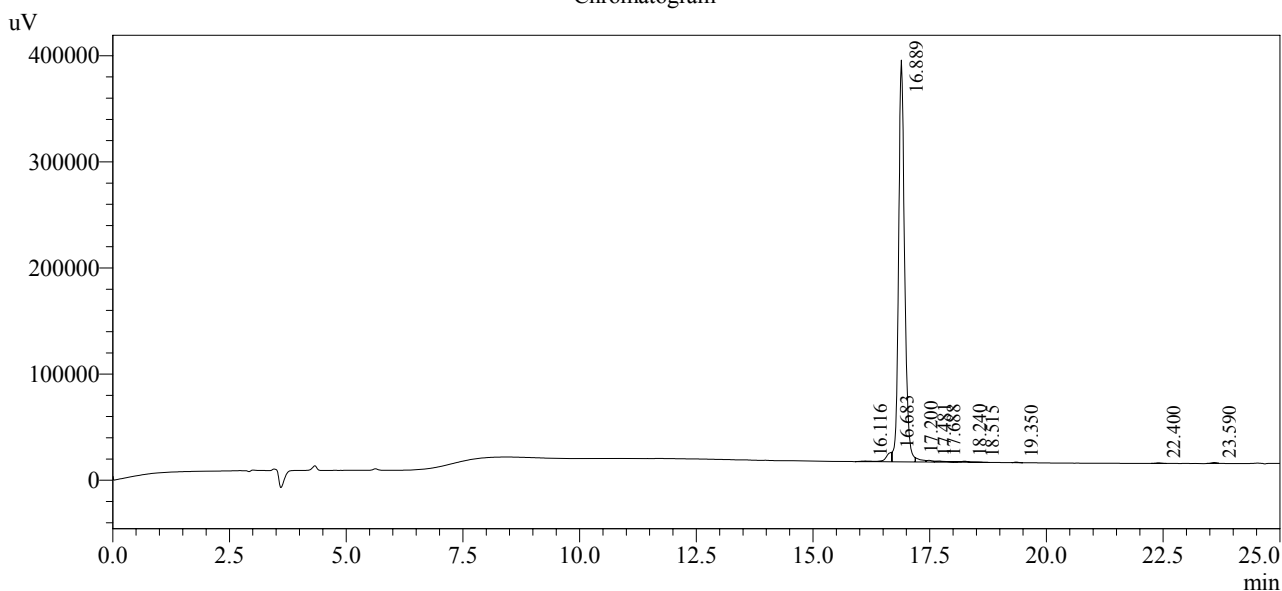

1 Det. A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.116	9793	525	0.275
2	16.683	74710	8936	2.096
3	16.889	3392334	378615	95.162
4	17.200	30418	3784	0.853
5	17.481	14164	1559	0.397
6	17.688	16271	1011	0.456
7	18.240	13230	1001	0.371
8	18.515	3512	364	0.099
9	19.350	3101	527	0.087
10	22.400	3631	451	0.102
11	23.590	3615	581	0.101
Total		3564780	397354	100.000