

Sample Name :PSA1 (141-150)  
 Cat No: RP20434  
 Lot No : E0643621A  
 Time Processed :9:40:02 AM  
 Month-Day-Year Processed :01/27/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010140

### <Chromatogram>

mV

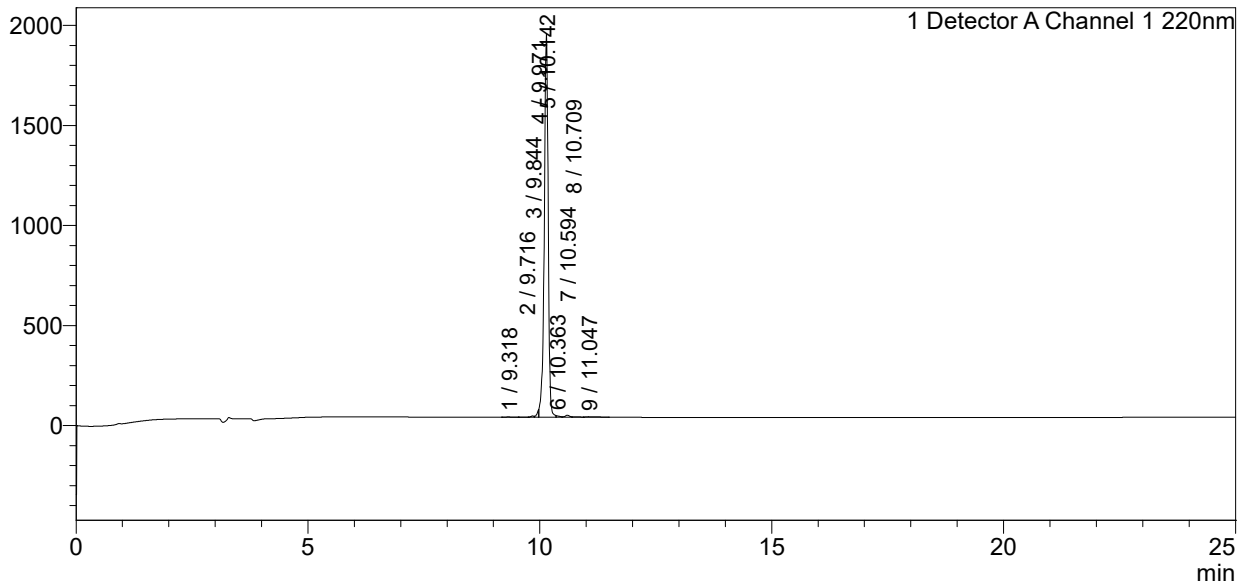

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.318	12080	1923	0.103
2	9.716	7175	890	0.061
3	9.844	31575	6330	0.269
4	9.971	97999	34162	0.834
5	10.142	11422896	1918080	97.190
6	10.363	37923	7322	0.323
7	10.594	71324	10616	0.607
8	10.709	24374	2697	0.207
9	11.047	47786	2763	0.407
Total		11753132	1984782	100.000