

Sample Name :Dynorphin A(1-13),porcine
 Cat No. :RP20492
 Lot No. :E0583720H
 Time Processed :15:50:29
 Month-Day-Year Processed :08/13/20

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
85.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

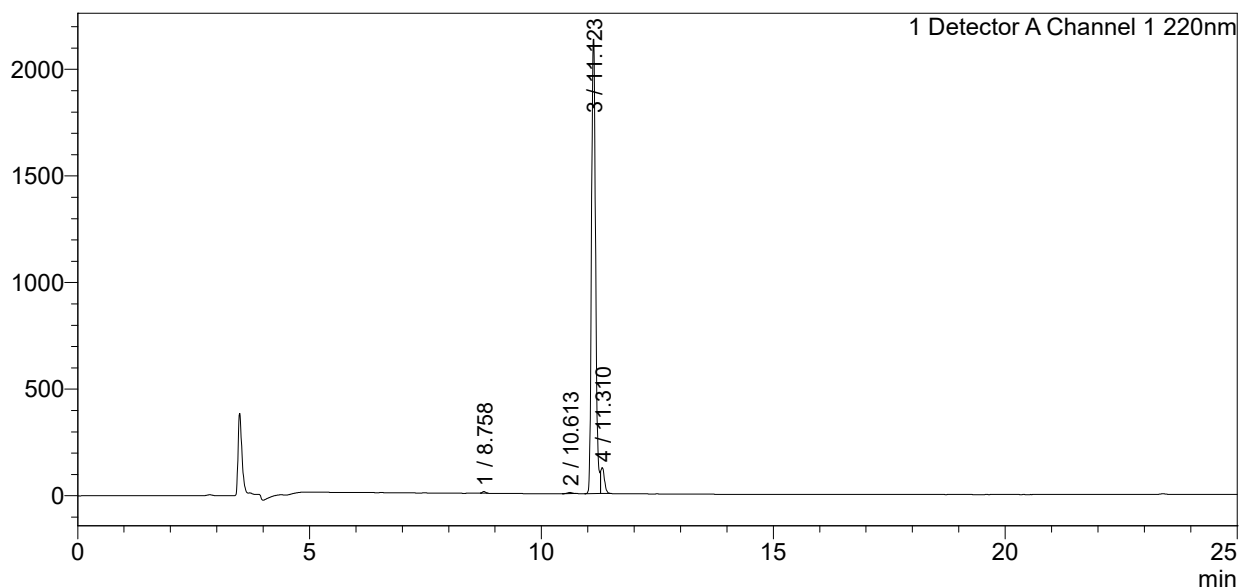

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.758	32712	7452	0.237
2	10.613	35975	5076	0.261
3	11.123	13121904	2129860	95.026
4	11.310	618230	122311	4.477
Total		13808821	2264699	100.000