

Sample Name : Gastrin-1, human
 Cat No. : RP12740
 Lot No. : PE2351706

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
31.00	Pumps	Pump B Conc.	95
31.01	Pumps	Pump B Conc.	5
40.00	Pumps	Pump B Conc.	5
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

<Chromatogram>

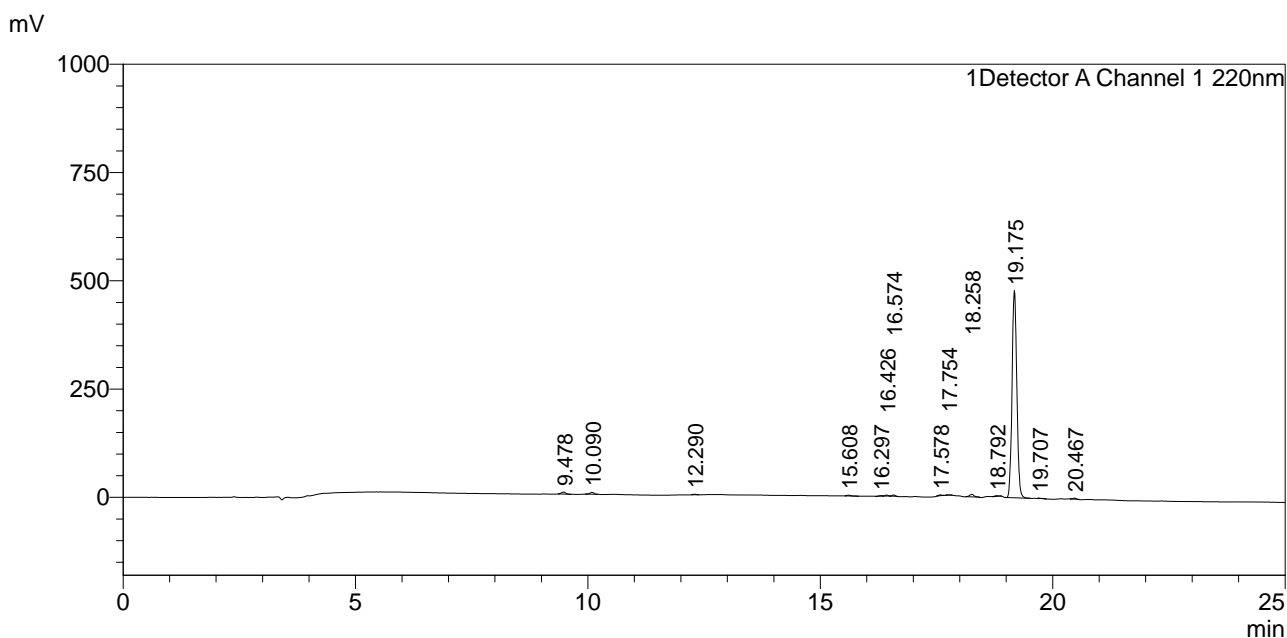

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.478	28005	4497	0.782
2	10.090	26761	4304	0.748
3	12.290	4557	1020	0.127
4	15.608	8756	1670	0.245
5	16.297	3411	904	0.095
6	16.426	9382	2219	0.262
7	16.574	13102	2921	0.366
8	17.578	9898	1925	0.277
9	17.754	2713	618	0.076
10	18.258	40984	6062	1.145
11	18.792	8527	1601	0.238
12	19.175	3408237	478407	95.217
13	19.707	2668	224	0.075
14	20.467	12433	2514	0.347
Total		3579433	508887	100.000