

Sample Name : SV40 large T antigen NLS  
Sample ID :U1295CJ080-1

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
Total Flow:1 ml/min  
Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

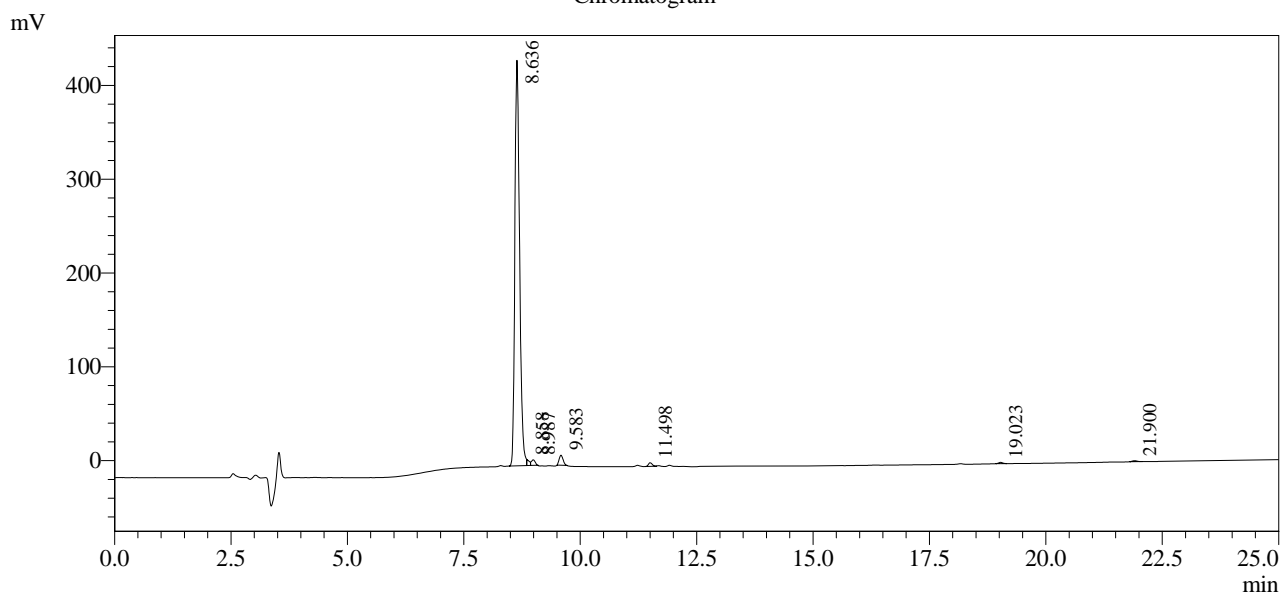

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.636	3046751	432143	95.088
2	8.858	24308	6250	0.759
3	8.987	33100	6005	1.033
4	9.583	62872	10640	1.962
5	11.498	21428	3846	0.669
6	19.023	8097	1317	0.253
7	21.900	7572	1033	0.236
Total		3204128	461234	100.000