

Sample Name :Corticotropin Releasing Factor, human, rat
 Cat. No. : RP10982
 Lot. No. : E0580120H
 Time Processed: 15:51:36

Month-Day-Year Processed :08/22/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

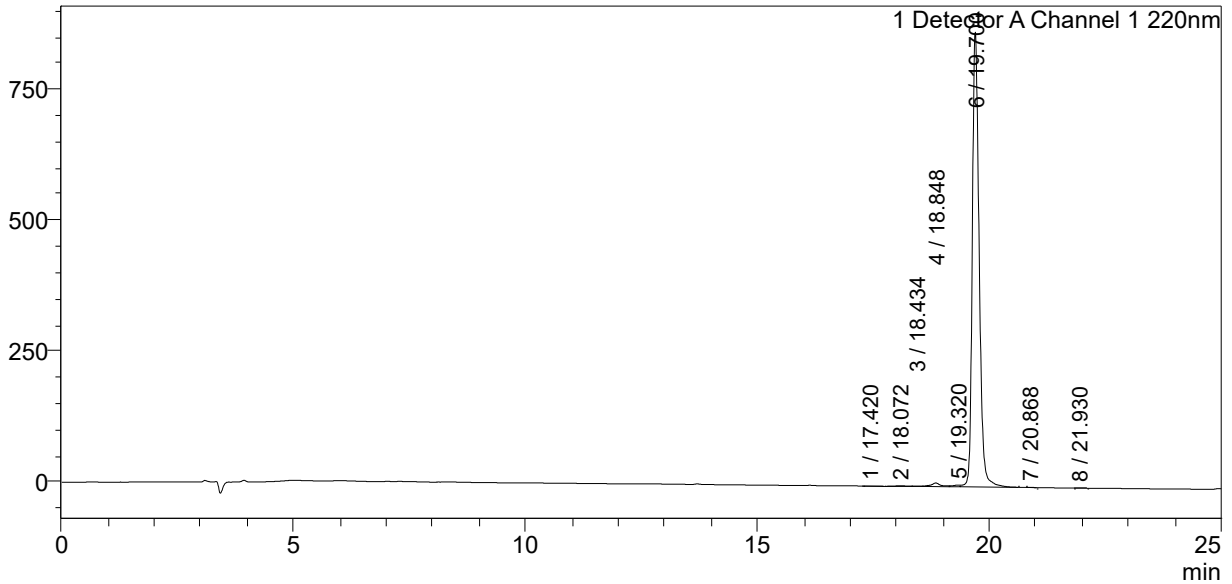

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	17.420	6793	406	0.075
2	18.072	23840	1306	0.263
3	18.434	10554	1005	0.116
4	18.848	107626	7020	1.185
5	19.320	37657	3385	0.415
6	19.700	8889002	868403	97.909
7	20.868	1433	209	0.016
8	21.930	1889	236	0.021
Total		9078794	881970	100.000