

Sample Name :Bradykinin (1-6)  
 Cat. No. :RP11132  
 Lot. No.:E4788919I  
 Time Processed :13:40:48  
 Month-Day-Year Processed :09/23/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

| Time  | Unit       | Command      | Value | Comment |
|-------|------------|--------------|-------|---------|
| 0.01  | Pumps      | Pump B Conc. | 5     |         |
| 25.00 | Pumps      | Pump B Conc. | 65    |         |
| 25.01 | Pumps      | Pump B Conc. | 95    |         |
| 31.00 | Pumps      | Pump B Conc. | 95    |         |
| 31.01 | Pumps      | Pump B Conc. | 5     |         |
| 40.00 | Pumps      | Pump B Conc. | 5     |         |
| 40.01 | Controller | Stop         |       |         |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

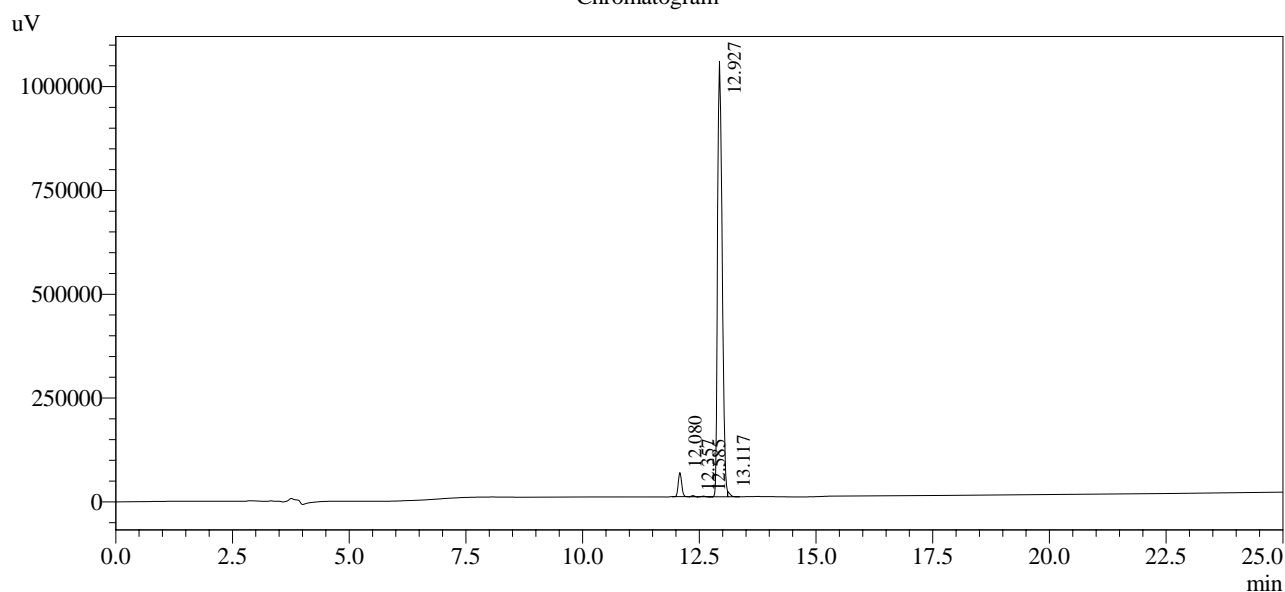

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

| Peak# | Ret. Time | Area    | Height  | Area %  |
|-------|-----------|---------|---------|---------|
| 1     | 12.080    | 294953  | 57954   | 3.881   |
| 2     | 12.357    | 13190   | 2656    | 0.174   |
| 3     | 12.585    | 6495    | 1439    | 0.085   |
| 4     | 12.927    | 7246910 | 1048793 | 95.350  |
| 5     | 13.117    | 38769   | 11548   | 0.510   |
| Total |           | 7600317 | 1122390 | 100.000 |