

Sample Name :Angiotensin II, human
 Cat. No. :RP11257
 Lot. No. :PE0261905

Time Processed :10:22:35 PM
 Month-Day-Year Processed :05/24/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ17010508

<Chromatogram>

mV

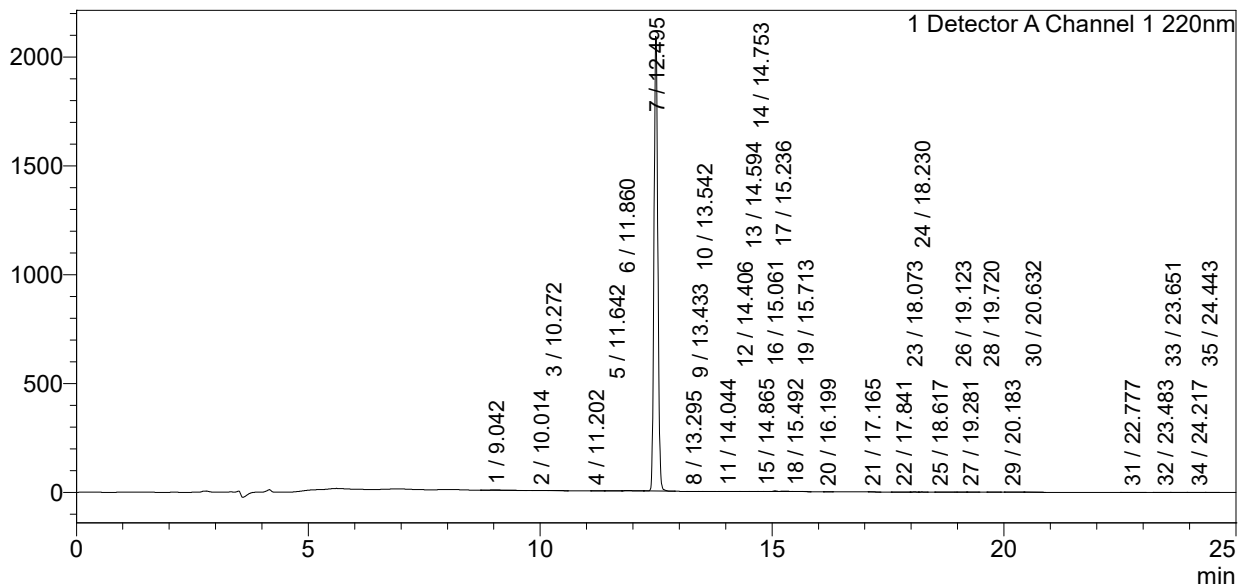

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.042	51816	1655	0.427
2	10.014	2122	216	0.018
3	10.272	5743	301	0.047
4	11.202	1077	112	0.009
5	11.642	8817	586	0.073
6	11.860	24879	2140	0.205
7	12.495	11913433	2090468	98.252
8	13.295	4633	487	0.038
9	13.433	2537	448	0.021
10	13.542	5231	568	0.043
11	14.044	4942	258	0.041
12	14.406	1837	247	0.015
13	14.594	6049	1057	0.050
14	14.753	1819	305	0.015
15	14.865	2139	328	0.018

Peak#	Ret. Time	Area	Height	Area%
16	15.061	20444	3304	0.169
17	15.236	26044	2232	0.215
18	15.492	6367	923	0.053
19	15.713	1877	402	0.015
20	16.199	2320	433	0.019
21	17.165	1134	187	0.009
22	17.841	3006	227	0.025
23	18.073	2450	431	0.020
24	18.230	2278	460	0.019
25	18.617	3122	154	0.026
26	19.123	1358	139	0.011
27	19.281	1691	182	0.014
28	19.720	1630	122	0.013
29	20.183	2216	155	0.018
30	20.632	2011	138	0.017
31	22.777	2113	133	0.017
32	23.483	2347	155	0.019
33	23.651	2002	180	0.017
34	24.217	2445	154	0.020
35	24.443	1489	126	0.012
Total		12125418	2109414	100.000