


Mass Spectrum

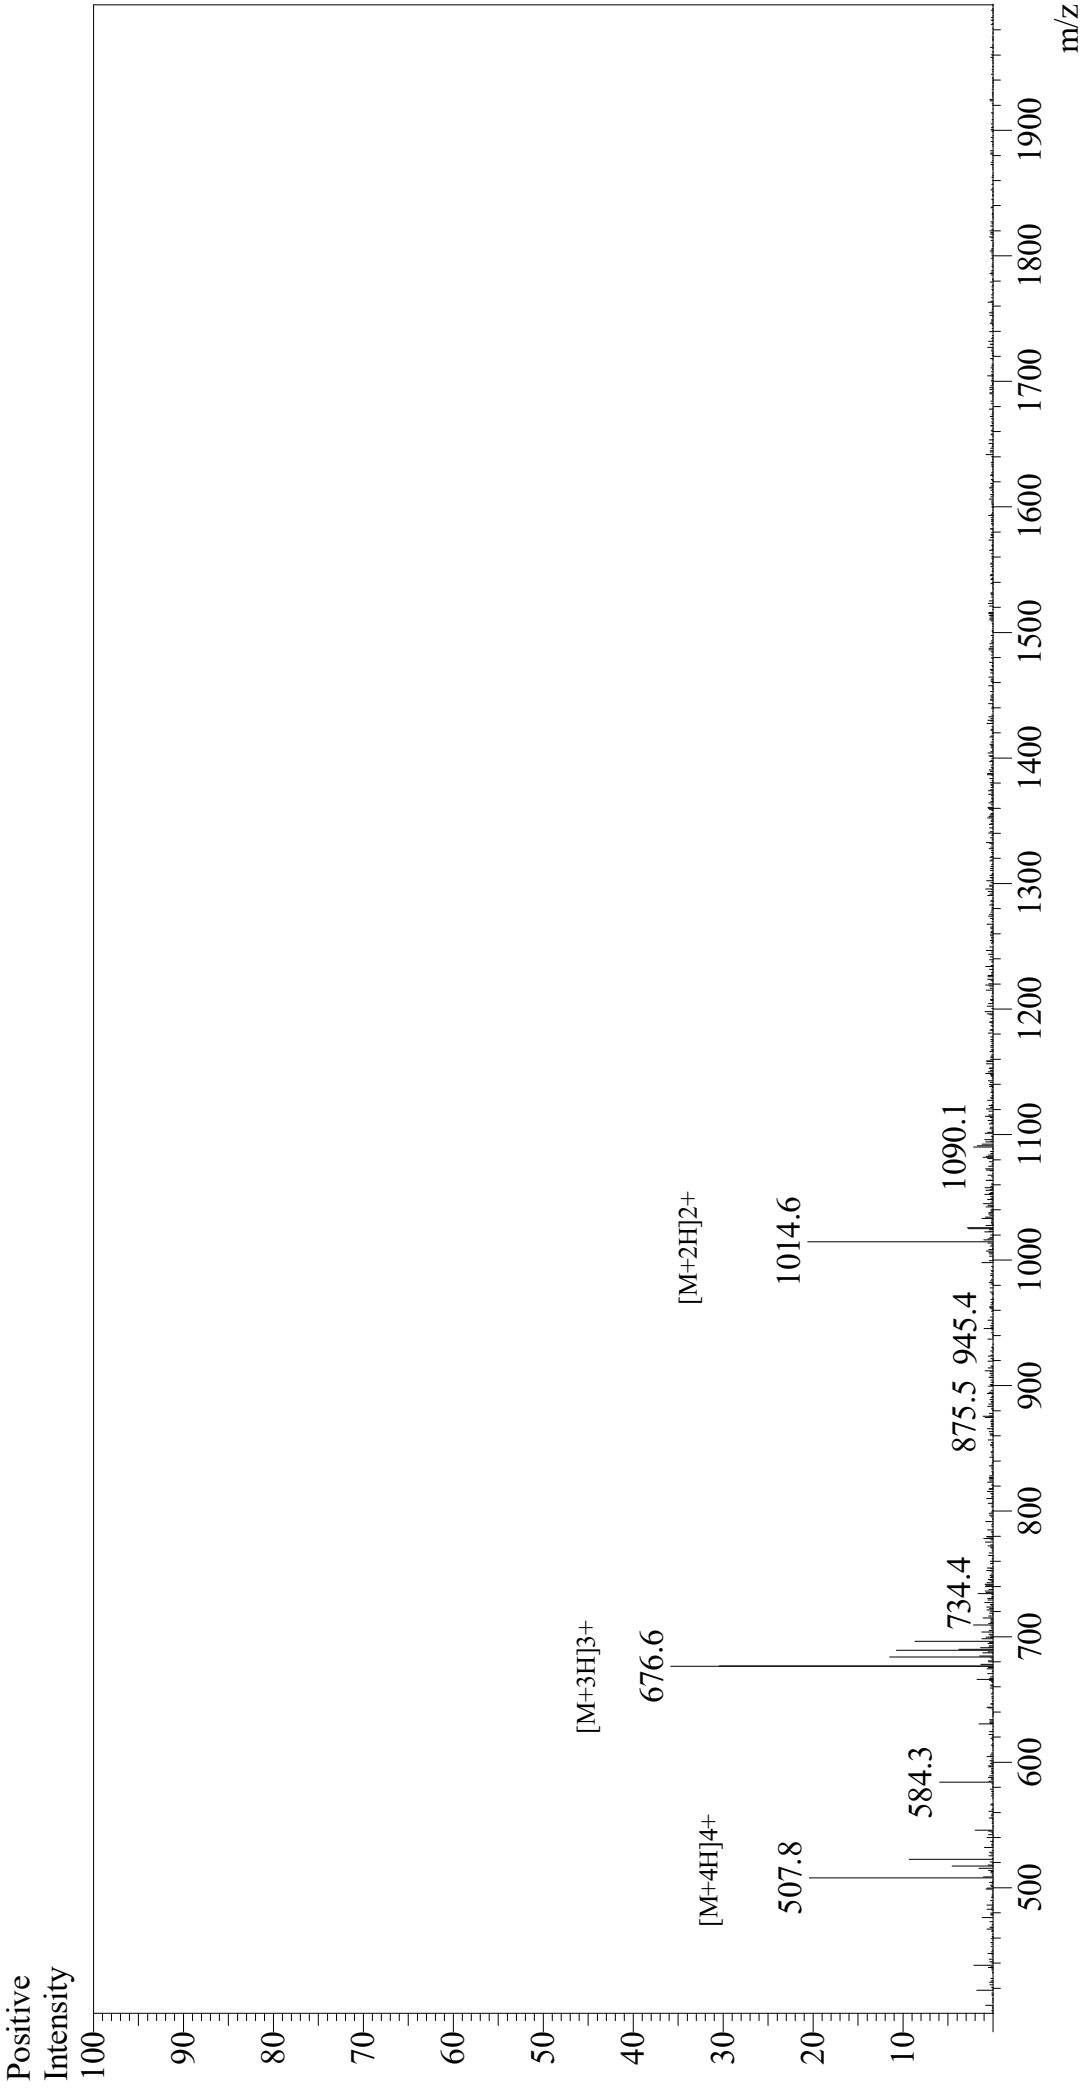

Sample Information
Month-Day Processed : 01/10/21
Time Processed : 11:12:32 AM
Injection Volume : 0.3
Sample Name : Apamin
Cat. No. : RP11002
Lot. No. : E7793520L
Theoretical MW : 2027.30
Observed MW : 2026.8

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H2O/50% MeOH