

Sample Name :[Leu5]-Enkephalin, amide
 Cat No. :RP10885
 Lot No. :E4771119I
 Time Processed :8:16:44
 Month-Day-Year Processed :09/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

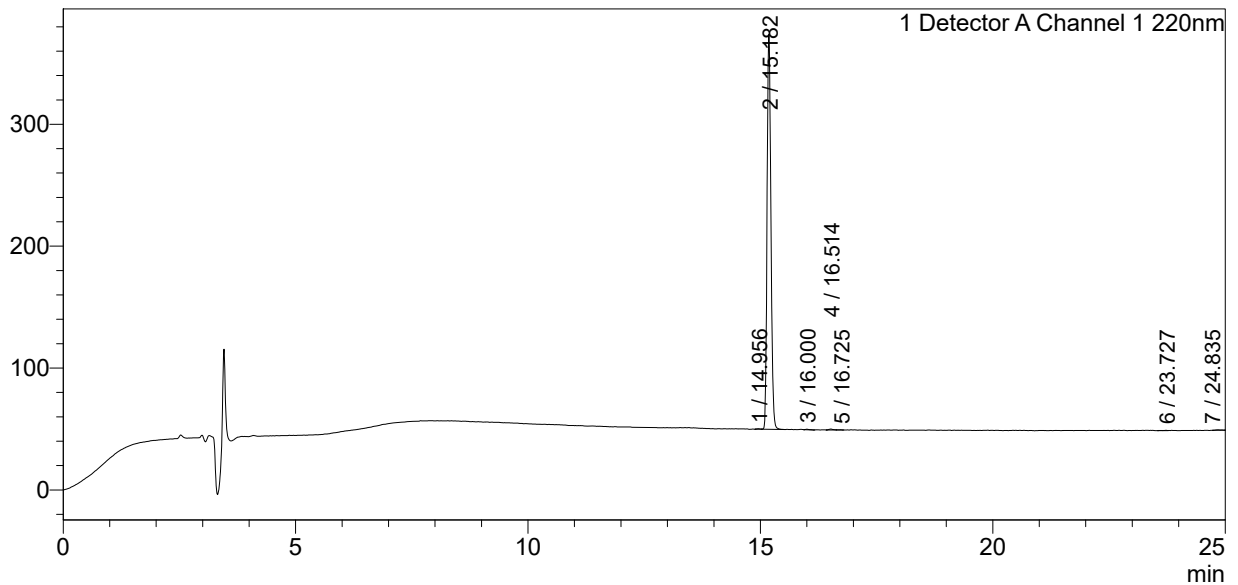

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.956	1783	404	0.095
2	15.182	1853393	323872	99.240
3	16.000	2389	453	0.128
4	16.514	4657	752	0.249
5	16.725	1040	203	0.056
6	23.727	1479	214	0.079
7	24.835	2843	328	0.152
Total		1867585	326226	100.000