


Mass Spectrum

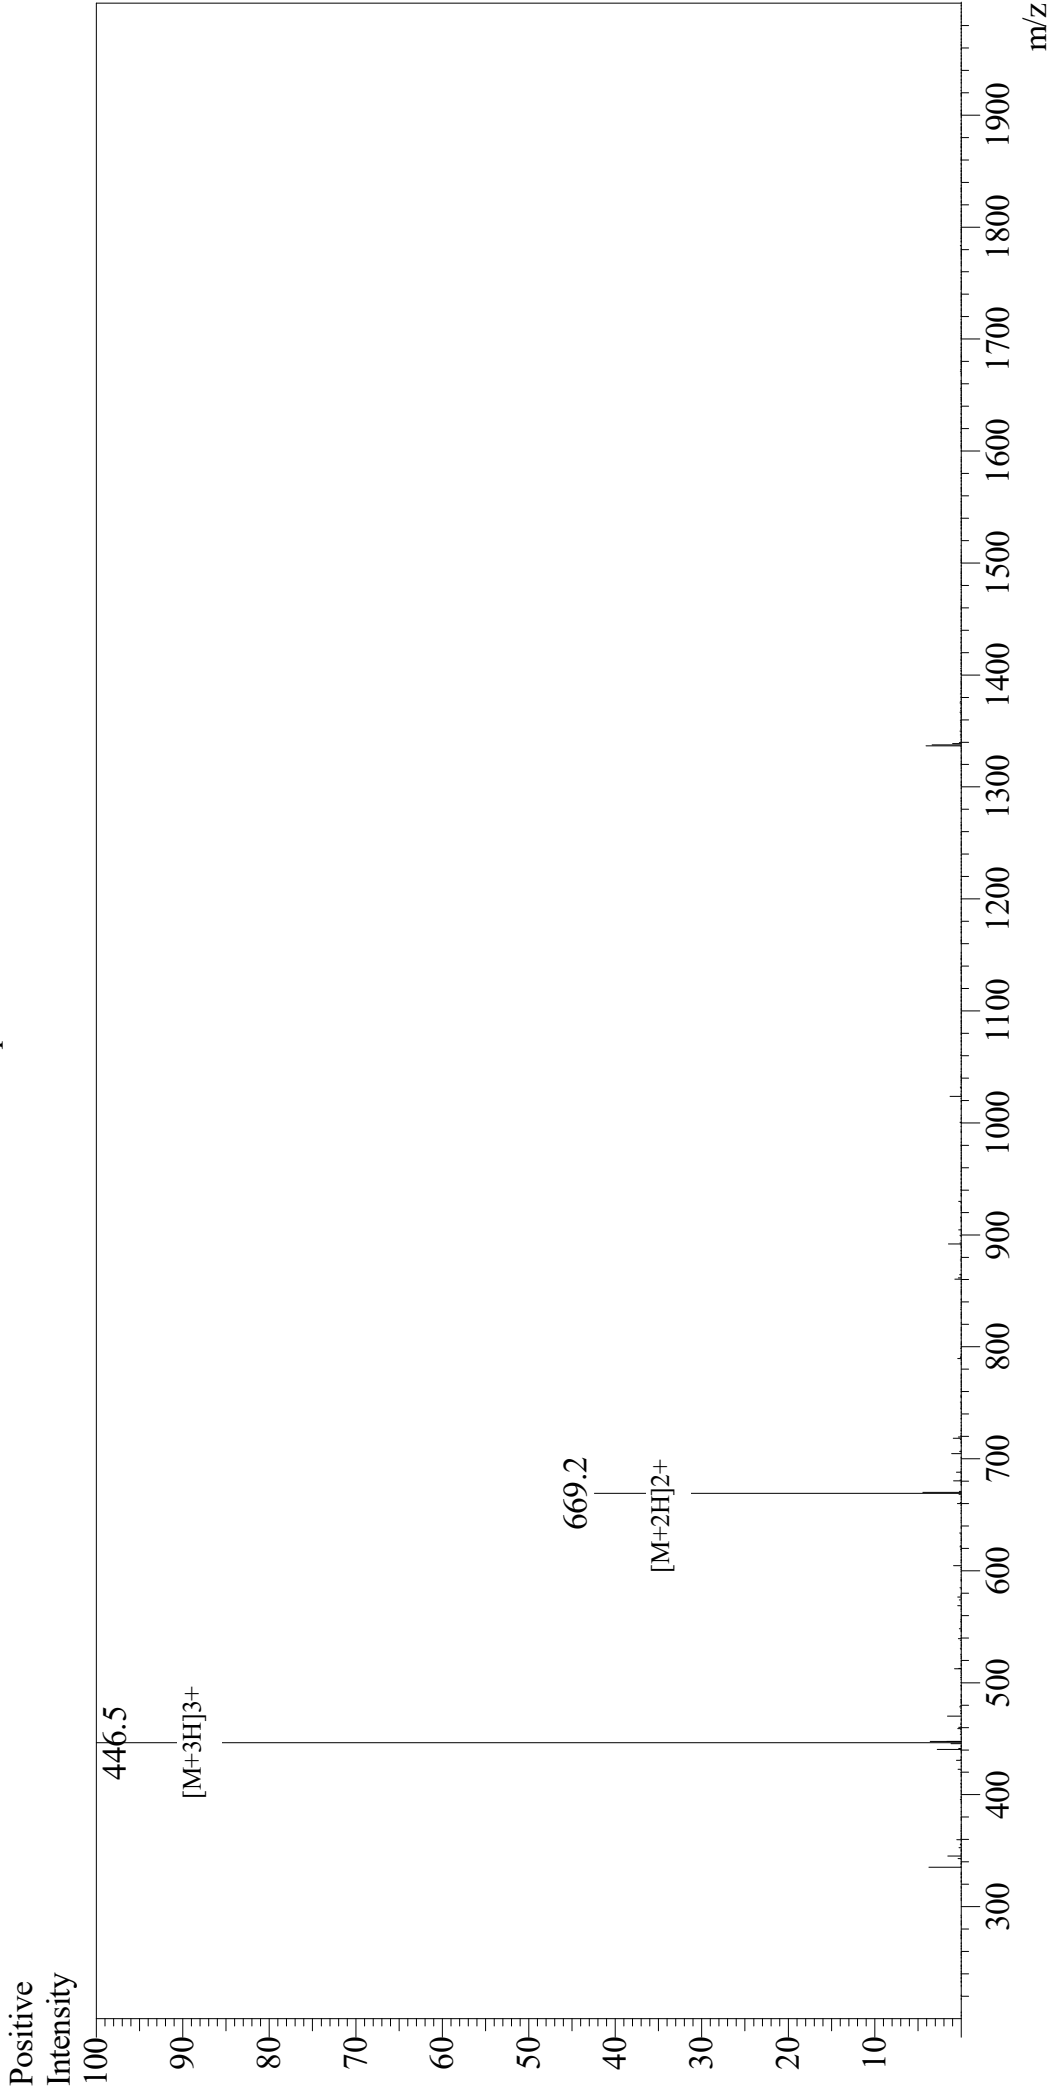

Sample Information

User :	Gary	Equipment	: GK11010007
Month-Day Processed :	09/28/19	Interface Bias	: +4.5kV
Time Processed :	11:53:03 AM	Drying Gas Flow	: 5 L/min
Injection Volume :	0.3	T.Flow	: 0.2ml/min
Sample Name :	Abl Cytosolic Substrate	B.conc	: 50% H ₂ O/50% MeOH
Cat No. :	RP19985		
Lot No. :	E4830719I		
Theoretical MW :	1335.61		
Observed MW :	1336.5		