

Sample Name :HPV16-E711-20 epitope
 Cat. No. : RP20285
 Lot. No. :PE8721902
 Time Processed :9:44:02
 Month-Day-Year Processed :03/02/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

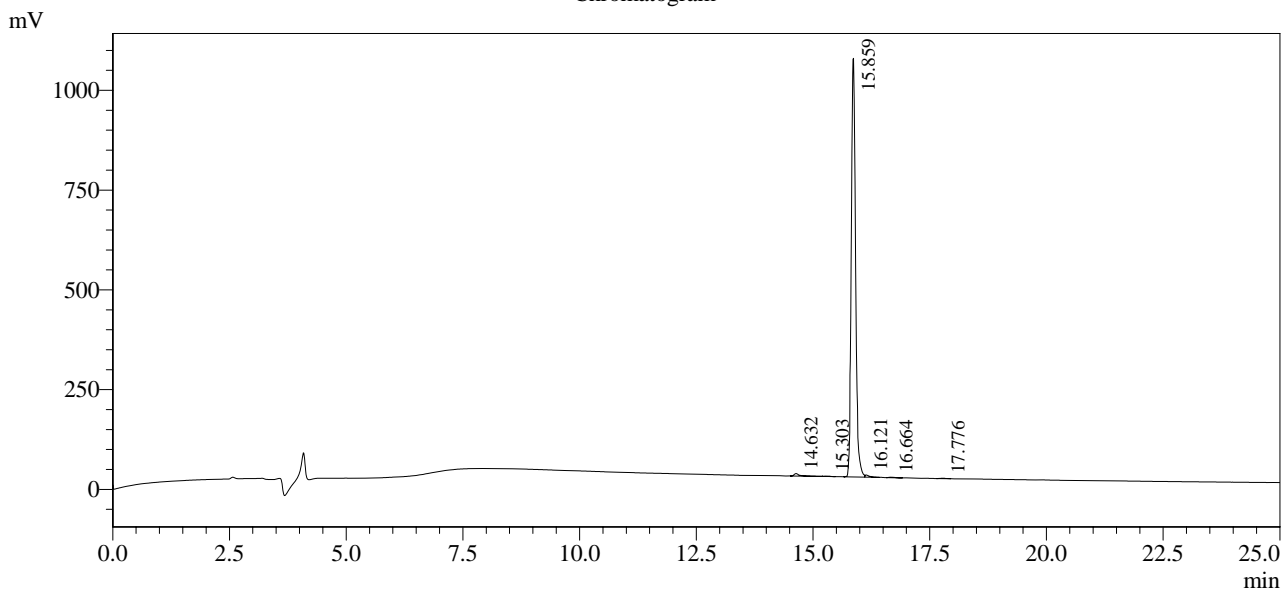

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.632	53260	6328	0.777
2	15.303	7798	989	0.114
3	15.859	6740943	1049029	98.359
4	16.121	32472	5263	0.474
5	16.664	11334	1375	0.165
6	17.776	7588	992	0.111
Total		6853395	1063976	100.000