

Sample Name :Hexa-His
 Cat. No. : RP11737
 Lot. No.: E7796619H
 Time Processed : 10:52:21
 Month-Day-Year Processed : 08/09/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	0	
25.00	Pumps	Pump A B.Conc	50	
31.00	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	0	
40.00	Pumps	Pump A B.Conc	0	
45.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

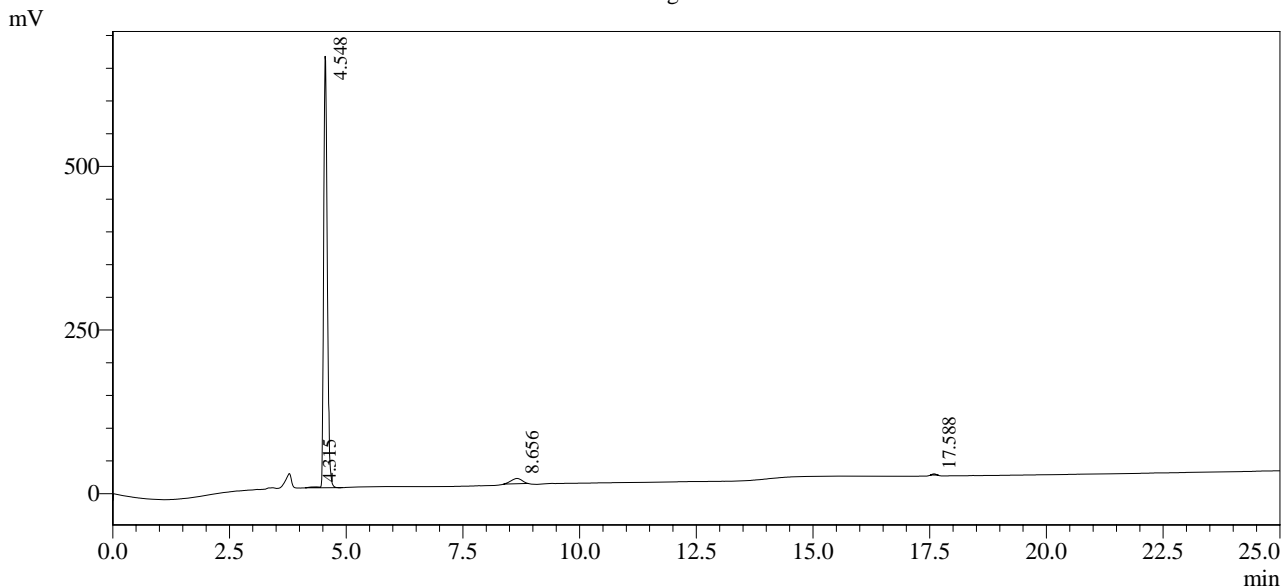

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	4.315	18065	1572	0.487
2	4.548	3552740	659298	95.688
3	8.656	131212	8065	3.534
4	17.588	10821	1873	0.291
Total		3712838	670808	100.000