

Sample Name :Bradykinin
 Cat No :RP11129
 Lot No :E4453621G
 Time Processed :23:39:27
 Month-Day-Year Processed :07/24/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

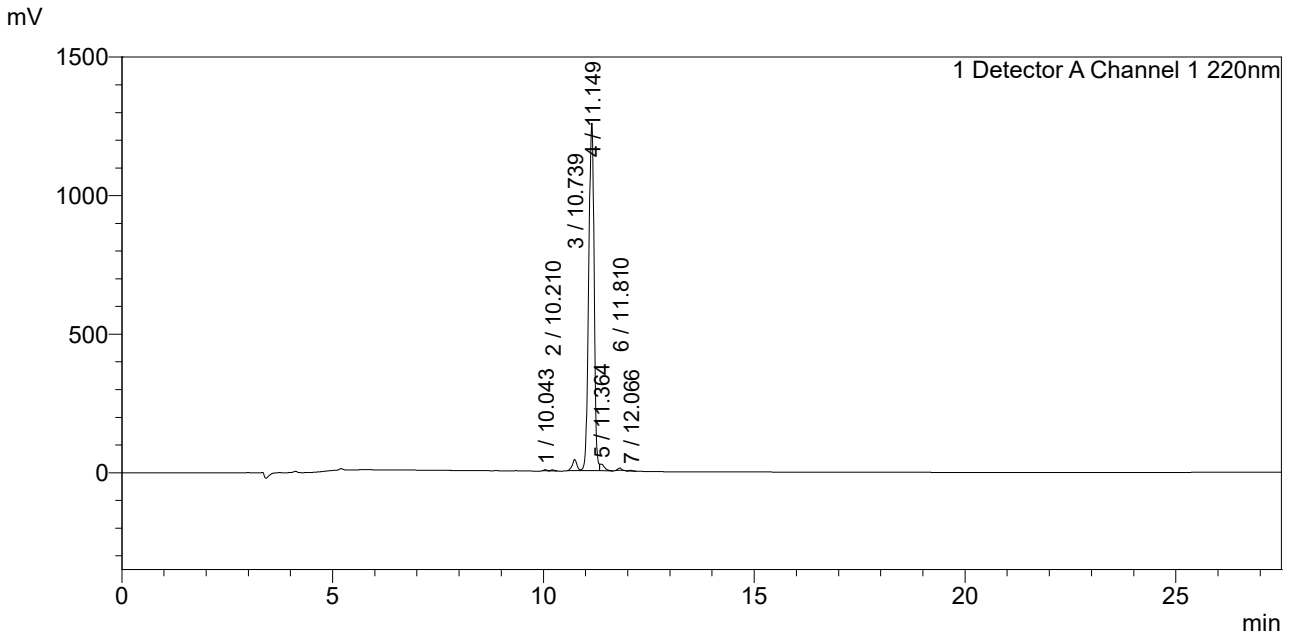

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.043	16342	3344	0.139
2	10.210	20036	3720	0.171
3	10.739	299700	39774	2.551
4	11.149	11175866	1254372	95.135
5	11.364	178403	23744	1.519
6	11.810	45576	8559	0.388
7	12.066	11431	2138	0.097
Total		11747353	1335652	100.000