

Sample Name: Phe-Met-Arg-Phe, amide  
 Cat. No. : RP10818  
 Lot. No. : E0428719H  
 Time Processed :7:31:16  
 Month-Day-Year Processed :08/28/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010014

<Chromatogram>

mV

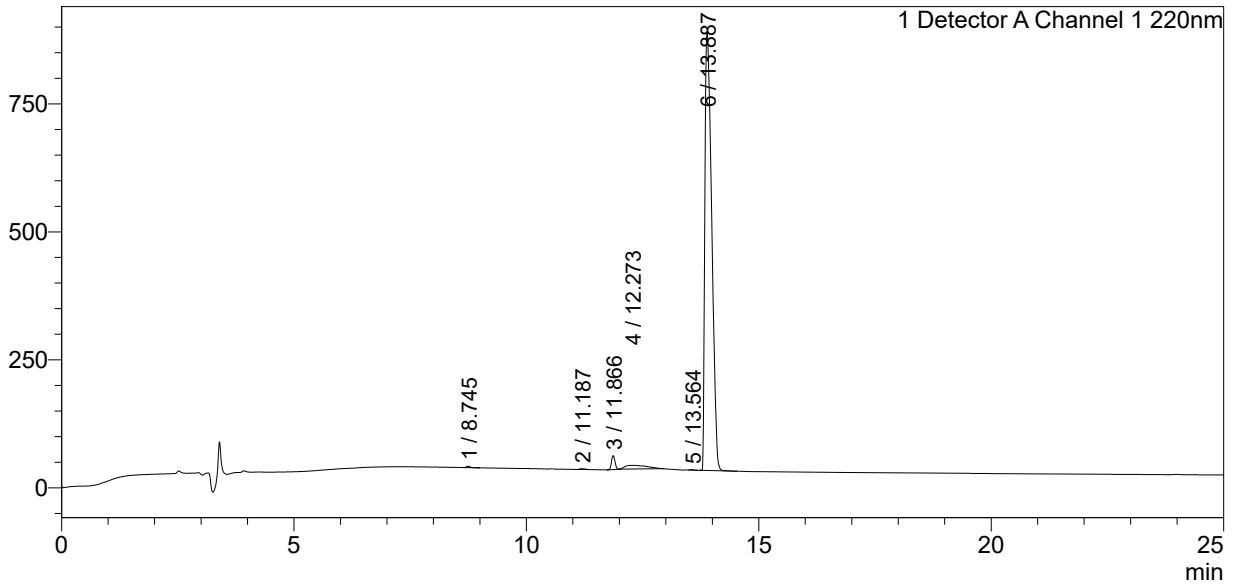

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.745	15319	2629	0.167
2	11.187	7623	1282	0.083
3	11.866	142328	27486	1.554
4	12.273	242777	7249	2.651
5	13.564	5723	1180	0.062
6	13.887	8743812	856198	95.482
Total		9157581	896023	100.000