

Sample Name : CEF14, EBV Rta Protein (28-37)
 Cat No.: RP20442
 Lot No.: E8424120D
 Time Processed : 12:05:21
 Month-Day-Year Processed : 04/23/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

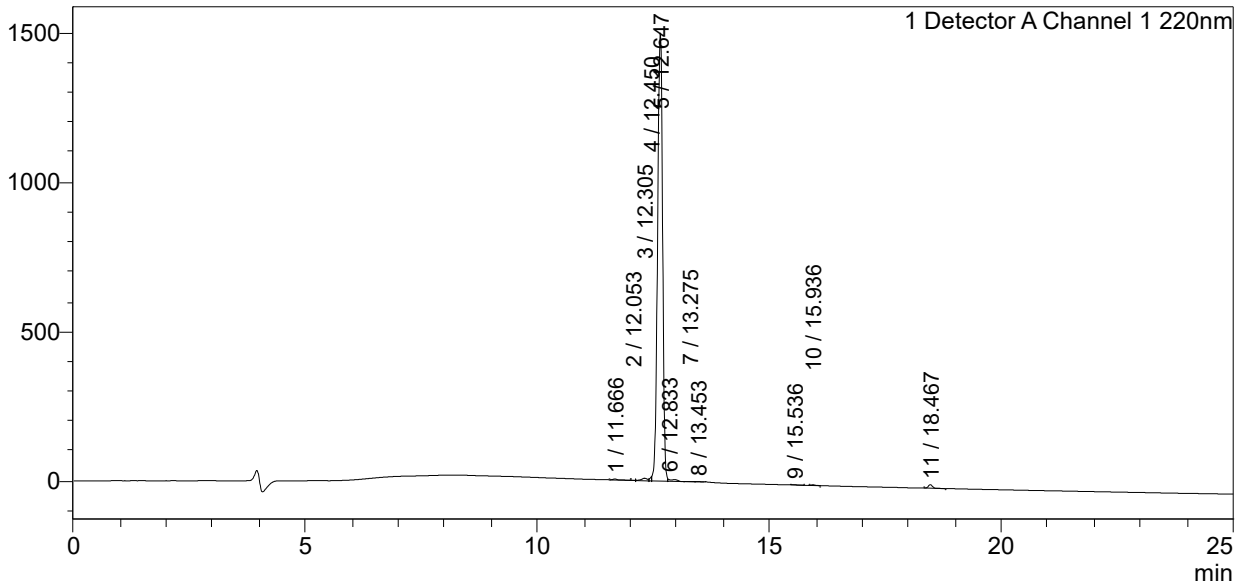

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.666	21887	3063	0.188
2	12.053	5402	815	0.046
3	12.305	70059	8469	0.603
4	12.450	40442	12533	0.348
5	12.647	11302391	1500032	97.252
6	12.833	72361	6138	0.623
7	13.275	12934	986	0.111
8	13.453	7244	1105	0.062
9	15.536	3104	555	0.027
10	15.936	12732	2173	0.110
11	18.467	73217	11984	0.630
Total		11621772	1547854	100.000