

Sample Name : TIP 39, Tuberoindubular Neuropeptide
 Cat No.: RP20232
 Lot No.: E4917419I
 Time Processed : 18:46:35
 Month-Day-Year Processed : 10/10/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

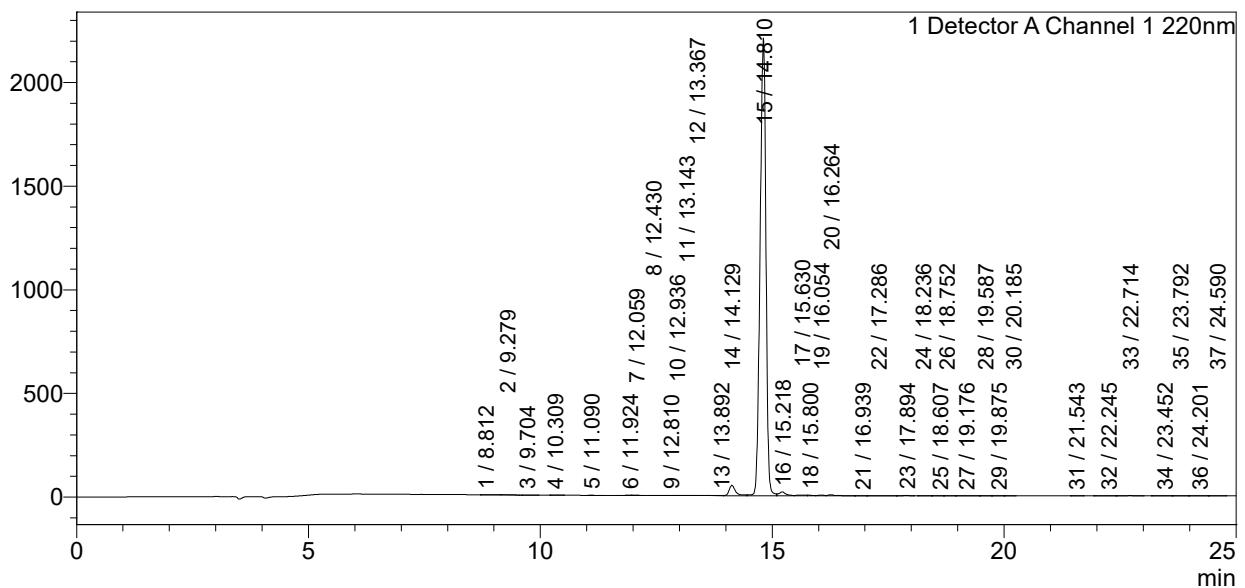

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.812	4705	277	0.023
2	9.279	4837	337	0.024
3	9.704	2492	231	0.012
4	10.309	2401	348	0.012
5	11.090	2902	250	0.014
6	11.924	7273	714	0.036
7	12.059	7798	904	0.039
8	12.430	2675	276	0.013
9	12.810	2143	336	0.011
10	12.936	3665	330	0.018
11	13.143	4112	440	0.020
12	13.367	2622	217	0.013
13	13.892	12050	1041	0.060
14	14.129	477379	49712	2.358
15	14.810	19295093	2208741	95.324

Peak#	Ret. Time	Area	Height	Area%
16	15.218	188664	18300	0.932
17	15.630	42991	3087	0.212
18	15.800	20194	2099	0.100
19	16.054	29924	3131	0.148
20	16.264	49067	5230	0.242
21	16.939	1197	131	0.006
22	17.286	8090	414	0.040
23	17.894	14548	1616	0.072
24	18.236	3666	269	0.018
25	18.607	4452	434	0.022
26	18.752	3640	408	0.018
27	19.176	3002	198	0.015
28	19.587	1769	167	0.009
29	19.875	1292	100	0.006
30	20.185	1071	93	0.005
31	21.543	1201	93	0.006
32	22.245	4970	330	0.025
33	22.714	15883	1500	0.078
34	23.452	4605	290	0.023
35	23.792	1499	146	0.007
36	24.201	4110	297	0.020
37	24.590	3598	281	0.018
Total		20241577	2302768	100.000