

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat
 Cat No.: RP11095
 Lot No.: E4557019K
 Time Processed : 10:47:18
 Month-Day-Year Processed : 11/17/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
31.00	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

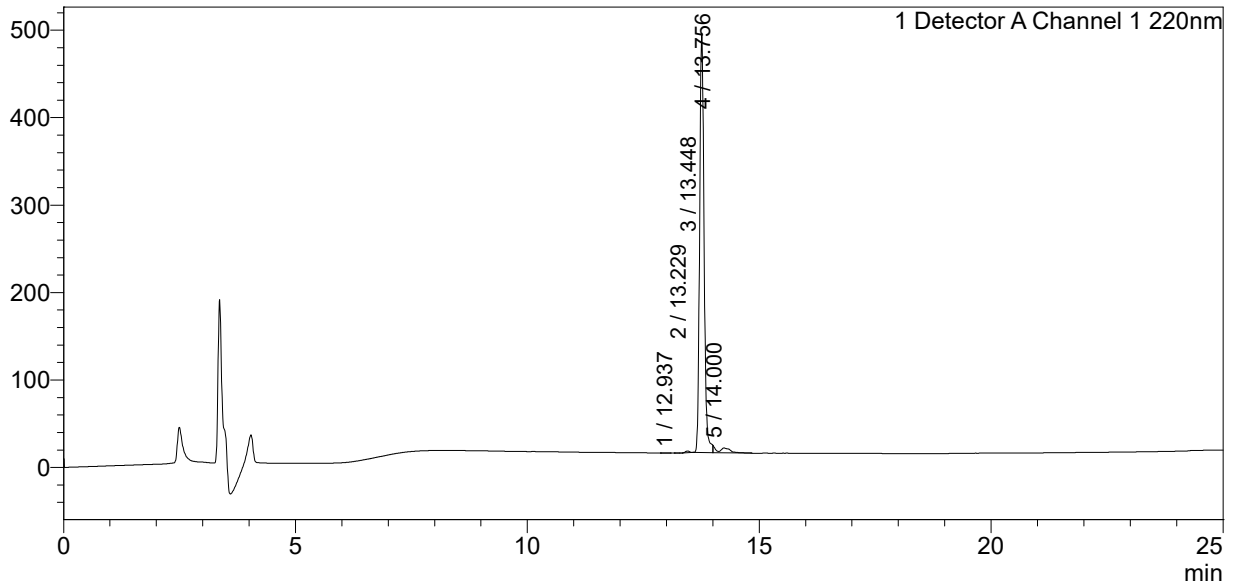

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.937	261	35	0.008
2	13.229	269	79	0.008
3	13.448	12351	2037	0.372
4	13.756	3197129	479974	96.377
5	14.000	107314	8618	3.235
Total		3317324	490743	100.000