

Sample Name:OVA Peptide (257-264)
 Cat No. :RP10611
 Lot No. :E4008121F
 Time Processed :21:37:56
 Month-Day-Year Processed :06/18/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

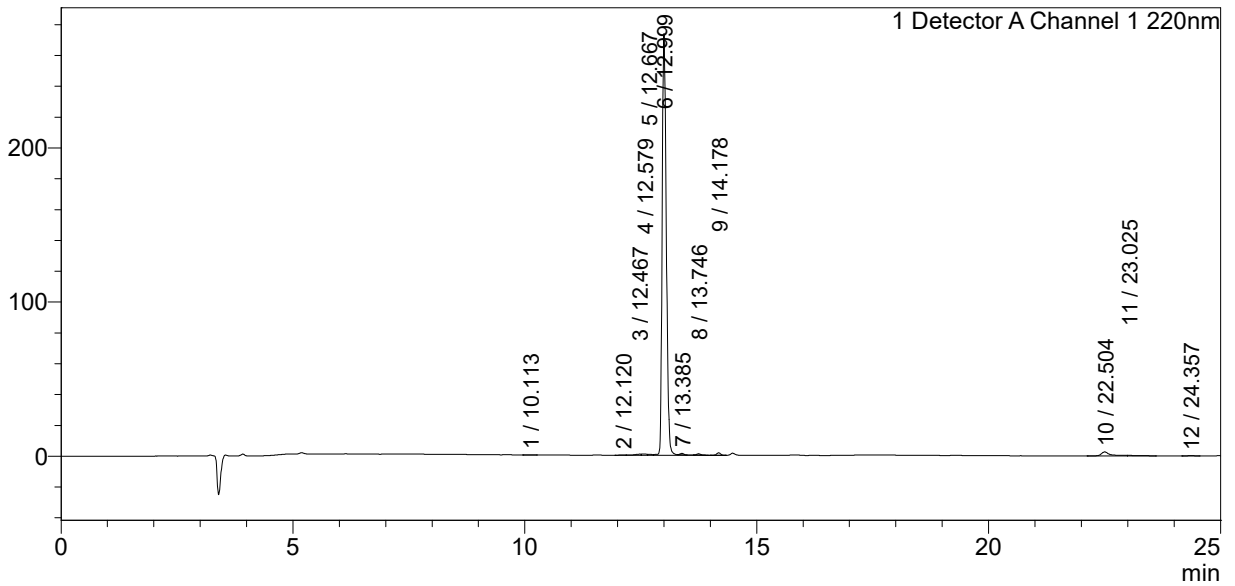

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.113	1006	84	0.056
2	12.120	1480	150	0.083
3	12.467	7514	707	0.421
4	12.579	6107	736	0.342
5	12.667	4395	707	0.246
6	12.999	1699144	273633	95.099
7	13.385	4748	937	0.266
8	13.746	5087	829	0.285
9	14.178	8950	1574	0.501
10	22.504	39362	2692	2.203
11	23.025	7379	405	0.413
12	24.357	1530	123	0.086
Total		1786702	282576	100.000